

Volume 69 Issue 2 October 2014 Pages 53-80 International Scientific Journal published monthly by the World Academy of Materials and Manufacturing Engineering

Overview and general ideas of the development of constructions, materials, technologies and clinical applications of scaffolds engineering for regenerative medicine

Leszek A. Dobrzański a,b

^a Institute of Engineering Materials and Biomaterials, Silesian University of Technology, ul. Konarskiego 18a, 44-100 Gliwice, Poland

b Institute of Advanced Materials Technology, ul. Wrocławska 37a, 30-011 Kraków, Poland Corresponding e-mail address: leszek.dobrzanski@polsl.pl

Received 23.09.2014; published in revised form 01.10.2014

ABSTRACT

Purpose: of this paper is the general presentation of the synergic utilisation of medical knowledge, tissue engineering and materials engineering for fabrication of functional substitutes of damaged tissues in the case of which medical indications show that classical prosthetics/implantation cannot be completely avoided, and that it is also appropriate to achieve natural ingrowth of the implanted elements into a living tissue in the implant area.

Design/methodology/approach: This refers to post-injury losses, post-resection losses, as well as those originating from operative treatment of cancerous tumours or inflammation processes. Implantable biomedical devices are currently aggregately considered to be medical bionic implants where bionics is understood as production and investigation of biological systems to prepare and implement artificial engineering systems which can restore the lost functions of biological systems.

Findings: The development of new hybrid technologies of bioactive and engineering materials for personalised scaffolds of tissues and bones requires a number of basic research and application work. They are presented numerous examples of the needs of the research for application of various bioactive and engineering materials, and their respective materials processing and tissue engineering technologies for manufacturing of the hybrid personalised implants and scaffolds.

Research limitations/implications: There are no reports in the references about an original concept presented by the Author of introduction of prosthetics/implantation and tissue engineering techniques for the purpose of natural ingrowth of the implanted elements into a living tissue in the implant area without having to use mechanical devices, at least in the connection (interface) zone of bone or organ stumps with prosthetic/implant elements.

Practical implications: They are open up vast possibilities for the application of the hybrid technologies of bioactive and engineering materials for personalized scaffolds of tissues and bones in accordance with the concept of the Author, presented in this paper.

Medical bionic implants encompass numerous solutions eliminating various disfunctions of a human organism, among other implants of the cardiovascular system (stents, vessel prostheses, heart valves, pacemakers, defibrillators), digestive system implants, neuron devices (implants and neuronal prostheses to the central (CNS) and peripheral nervous system (PNS), the cochlea, retina), orthopaedic prostheses (bone grafts, bone plates, fins and other connecting and stabilising devices, including screws applied in the area of ankles, knees and hands, bars and pins for stabilising fractured limbs), screws and plates in skull-jaw-face reconstructions, dental implants, and also scaffolds of bones and tissues in tissue engineering.

Originality/value: The Author's idea for the embracing hybrid technologies of bioactive and engineering materials with titanium alloys including personalised scaffolds of tissues and bones will be created. It is also a challenge to achieve a synergy of clinical effects obtained with classical prosthetics/implantation of large lost post-injury or post-resection recesses together with the use of achievements in advanced tissue engineering methods at least in the interface zone of bone or organ stumps with prosthetic elements/implants.

Keywords: Regenerative medicine; Scaffolds engineering; Tissue engineering; Prosthetics; Implantation; Medical bionic implants; Interface zone

Reference to this paper should be given in the following way:

L.A. Dobrzański, Overview and general ideas of the development of constructions, materials, technologies and clinical applications of scaffolds engineering for regenerative medicine, Archives of Materials Science and Engineering 66/2 (2014) 53-80.

GENERAL REVIEW

1. Introduction

The dynamic growth of cases of organ or tissue loss or damage in the human population due to post-injury losses, post-resection losses, as well as those originating from operative treatment of cancerous tumours or inflammation processes and as a result of other disorders and the related necessity to replace or supplement such organs or tissues aimed at the prevention of biological and social degradation of patients and restoration of their living functions, either normal functions or such acceptably similar to normal, constitutes a significant and costly problem of modern medicine. It is hard to overestimate, nowadays, the achievements of modern implantology, where courage, imagination and knowledge of doctors supported by accomplishments of engineers have, on a global scale, given many people an opportunity to return to their normal or quasi-normal conditions of functioning, and very often to have their health restored after experiencing severe injuries or losses, and also other disorders. One of the challenges for regenerative medicine is to reconstruct sections of bone losses in maxillo-facial surgery, restorative dentistry, laryngology, including otolaryngology, orthopaedics and traumatology, and to supplement soft tissues, e.g. in case of oesophagus and blood vessels prosthetics/implantation, where in particular bone or organ stumps are not in contact. This refers to post-injury losses, post-resection losses, as well as those originating from operative treatment of cancerous tumours or inflammation processes. Implantable biomedical devices are currently aggregately considered to be medical bionic implants where bionics is understood as production and investigation of biological systems to prepare and implement artificial engineering systems which can restore the lost functions of biological systems [1]. In general, medical bionic implants encompass numerous solutions eliminating various dysfunctions of a human organism, among other implants of the cardiovascular system (stents, vessel prostheses, heart valves, pacemakers, defibrillators), digestive system implants, neuron devices (implants and neuronal prostheses to the central (CNS) and peripheral nervous system (PNS), the cochlea, retina), orthopaedic prostheses (bone grafts, bone plates, fins and other connecting and stabilising devices, including screws applied in the area of ankles, knees and hands, bars and pins for stabilising fractured limbs), screws and plates in skull-jaw-face reconstructions, dental implants, and also scaffolds of bones and tissues in tissue engineering [1].

It is expected that the development rate of each of the existing **global medical products market** segments will differ depending on multiple objective factors. On one hand, it is associated with civilisational progress, longer life expectancy, many societies becoming richer, including definitely the Polish society. The global biomaterials market was valued at USD 25,277.8 million in 2012

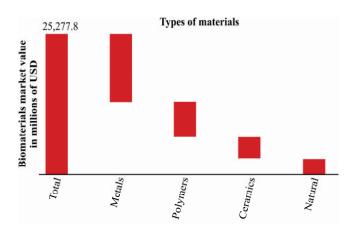


Fig. 1. The global biomaterials market value in 2012; according to data from [2]

(Fig. 1) [2]. On the figure is presented the division of the biomaterials for the main group of materials. The global orthopaedic devices market was valued at USD 29.2 billion in 2012 (Fig. 2) [3]. Orthopaedic devices are used to restore skeletal structure and joint movements in various types of fractures, abnormal growth of bones, soft tissue damage, trauma or other deformities. The statistics of the Central Statistical Office (GUS) show that healthcare expenditures in Poland are constantly on the rise in billions of PLN (Fig. 3) (lines on the figure above show expenses for: current expenses, related investments - no-investment and investment expenses). The radar chart (Fig. 4) [4] shows that public spendings, as a share in overall healthcare spendings, in Poland in 2011 are merely about 15% lower than in the top ranking OECD countries. It should nevertheless be admitted that challenges in Poland in this context are very serious considering huge civilisational backwardness in this field. The OECD's analyses presented in the same paper show that overall healthcare expenditures, by purchasing power per capita in thousands of USD in OECD countries in 2011 (Fig. 5), rank Poland on one of the last positions among such countries. On the other hand, the development rate of segments of the medical products market is linked to sharp development of civilisational diseases, including cancer. The incidence rate of malignant cancers in Poland has been regularly rising from 124,407 in 2005 to 138,227 in 2010 [5]. The number of traffic accidents' victims has been growing systematically, as well. The European Commission informs in its Press Announcement of 19 March 2013 that, according to the Eurostat's data for 2011, Poland has a worryingly unfortunate first position in the European Union with 109 fatalities per million inhabitants, while the same figure for the Great

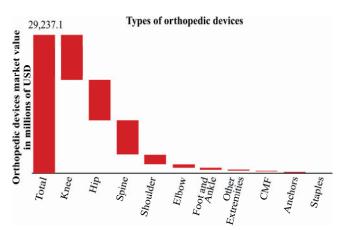


Fig. 2. The global orthopaedic devices market value in 2012; according to data from [3]

Britain is lowest in the European Union of 31, and average decline in this indicator in Latvia and Estonia is 10%, is 543, which is the highest for the European Union, whilst in, e.g. Estonia, Finland and the Netherlands is below 20. Followed by this, almost proportionally, the number of people injured in such accidents and requiring usually **long-lasting medical care grows**. Along with the intensification sports activity, especially among young people, and with promotion of leisure practise of sports by propagating healthy lifestyle, more and more mature people start to practise sports, which is inherent to the **growing number of sports accidents** and the related serious bodily injuries of many people on a global scale. Globally, rise in aging

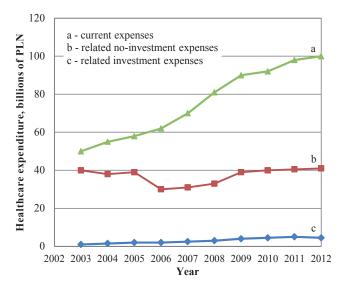


Fig. 3. The changes of the healthcare expenditures in Poland; according to data from [4]

Volume 69 Issue 2 October 2014

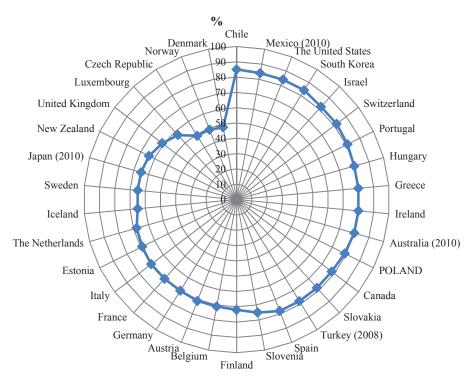


Fig. 4. The public spendings, as a share in overall healthcare spendings in 2011 in OECD countries; according to data from [4]

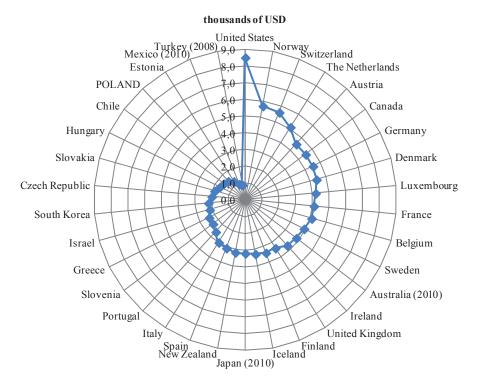


Fig. 5. The overall healthcare expenditures, by purchasing power per capita in 2011 in OECD countries; according to data from [4]

population plays a major role in increasing the incidence of sports injuries as aging diminishes body whilst it goes up by 4% on average annually in Poland. Analogously, the number of fatalities in railway accidents functions and movements which makes the body more prone to injuries. For instance, according to the European Injury Database (EU IDB) catalogue, annually on an average 6.1 million people in the European Union are treated in hospitals for sports injuries. Patients' healthcare expectations are also growing, and economic aspects at the domestic scale call for efficient elimination of disabilities, in particular motoric disabilities and restoring previously handicapped persons to physical fitness and usually most often to full or at least partial professional activity, which considerably lessens pressure on the diminishing social insurance funds.

In the paper the state-of-the-art of the constructions, materials, technologies, applications and clinical experiences of the scaffolds engineering for regenerative medicine is presented. Furthermore the Author's idea of the synergy of classical prosthetics/implantation of bone and organ post-injury or postresection losses together with the methods of tissue engineering in the connection (interface) zone of bone or organ stumps with prosthetic elements/ implants, call for the use of porous and high-strength nongraded metal and/or composite and/or polymer materials (which is strongly, but not exclusively, dependent on the specificity of the clinical application) together with using at the same time biodegradable materials for tissue scaffolds is presented. Numerous actions are undertaken in general by the Author in his own research,

which most generally requires a differentiated methodological approach, materials and technologies used and clinical application methods, concerning the filling of bone losses, joint cartilage cells, oesophagus and/or blood vessels, dental and skin restorations. The lack of procedures for solving synergistically the above issues in the case it is not possible to apply exclusively tissue engineering methods, for instance due to extensive bone or tissue losses, but also for other reasons, substantiates the appropriateness of addressing the challenges outlined by the Author. The aforementioned concept of the synergic use, for this purpose, of the existing achievements in surgery and regenerative medicine in scope of prosthetics/ implantation in treatment of the above-mentioned civilisational diseases and their effects, production engineering and materials engineering in scope of design and manufacture of prostheses/implants with different engineering materials and tissue engineering in scope of selection of materials and scaffold fabrication technologies, has been outlined in the earlier own works and projects of the Authors and another Polish researchers [6-21]. At the same time, accomplishments and clinical experiences of distinguished surgeons confirm the necessity to address the said research and implementation path due to urgent needs experienced immediately at the operating table [22-27], and the accomplishments of the tissue bank workers confirm, on the other hand, it is possible to use their own achievements in the field of tissue engineering for this idea [28-31], and that it is also possible to use different highlyspecialised technologies, considering the outcomes of the theoretical Author's own works and another Polish researchers attained in this field to date [10, 11, 32-48].

The objective of the paper is the general presentation of the synergic utilisation of medical knowledge, tissue engineering and materials engineering for fabrication of functional substitutes of damaged tissues in the case of which medical indications show that classical prosthetics/ implantation cannot be completely avoided, and that it is also appropriate to achieve natural ingrowth of the implanted elements into a living tissue in the implant area. For this reason, Author's idea for the embracing hybrid technologies of bioactive and engineering materials with titanium alloys including personalised scaffolds of tissues and bones will be created. It is also a challenge to achieve a synergy of clinical effects obtained with classical prosthetics/implantation of large lost post-injury or postresection recesses together with the use of achievements in advanced tissue engineering methods at least in the interface zone of bone or organ stumps with prosthetic elements/implants.

2. Description of the state of research of the materials and technologies applied in the scaffolds engineering for regenerative medicine

The dynamic growth of cases of organ or tissue loss or damage in the human population due to post-injury losses, post-resection losses, as well as those originating from operative treatment of cancerous tumours or inflammation processes and as a result of other disorders and the related necessity to replace or supplement such organs or tissues aimed at the prevention of biological and social degradation of patients and restoration of their living functions, either normal functions or such acceptably similar to normal, constitutes a significant and costly problem of modern medicine. It is hard to overestimate, nowadays, the achievements of modern implantology, where courage, imagination and knowledge of doctors supported by accomplishments of engineers have, on a global scale, given many people an opportunity to return to their normal or quasi-normal conditions of functioning, and very often to have their health restored after experiencing severe injuries or losses, and also other disorders. One of the challenges for regenerative medicine is to reconstruct sections of bone losses in maxillo-facial surgery, restorative dentistry, laryngology, including otolaryngology, orthopaedics and traumatology, and to supplement soft tissues, e.g. in case of esophagus and blood vessels prosthetics/ implantation, where in particular bone or organ stumps are not in contact. This refers to post-injury losses, postresection losses, as well as those originating from operative treatment of cancerous tumours or inflammation processes. Implantable biomedical devices are currently aggregately considered to be medical bionic implants where bionics is understood as production and investigation of biological systems to prepare and implement artificial engineering systems which can restore the lost functions of biological systems [1]. In general, medical bionic implants encompass numerous solutions eliminating various disfunctions of a human organism, among other implants of the cardiovascular system (stents, vessel prostheses, heart valves, pacemakers, defibrillators), digestive system implants, neuron devices (implants and neuronal prostheses to the central (CNS) and peripheral nervous system (PNS), the cochlea, retina), orthopaedic prostheses (bone grafts, bone plates, fins and other connecting and stabilising devices, including screws applied in the area of ankles, knees and hands, bars and pins for stabilising fractured limbs), screws

and plates in skull-jaw-face reconstructions, dental implants, and also scaffolds of bones and tissues in tissue engineering [1].

Diagnostic methods of medical imaging, including Advanced Computed Tomography (ACT) including X-ray tomography, CAT Computerized Axial Tomography, HRCT High Resolution Computed Tomography, MSCT Multi-Slice Computed Tomography or MDCT Multi-row-Detector Computed Tomography, and also PET Positron Emission Tomography and MRI Magnetic Resonance Imaging [49], modelling and design methods of Computer Aided Design/Manufacturing CAD/CAM [50] and Rapid Manufacturing (RM) and Rapid Prototyping (RP) methods could be employed to accomplish the assumptions of this idea to enable the connection (interface) of bone or organ stumps with prosthetic elements/implants for their synergic manufacturing [51-53]. The solutions proposed by the Author strive to achieve bioactive connections, as most advantageous in terms of bond strength, which are formed between bone tissue and implants/scaffolds made or coated with bioactive materials, considerably improving the stability and durability of connection, especially for porous scaffolds/implants. Another acceptable approach is a very durable biological connection characteristic for porous implants/scaffolds whereby the bone tissue grows through the material pores and is mechanically "anchored" in the bone. Porous resorbable bioglass may be used for scaffold fabrication [47, 54], e.g. from the CaO-SiO₂-P₂O₅ system, Hench bioglass [55], produced both, with classical melting methods and with sol-gel methods, and also bioglass from the SiO₂-Al₂O₃ system endowed with silver [56], due to their biocompatibility [57] and bacteriocidity [58], and with pore walls coated with hydroxy carbonate apatite (HCA) [48], ensuring enhanced activity of osteoblasts [59] and expression of genes connected with bones [60]. The formation methods of porous structures from ceramic materials, in particular such as aluminium oxide, zirconium oxide, calcium carbonate, hydroxyapatite (HA), titanium oxide, include casting of sections from mass containing a fine-grained ceramic material with additives facilitating foaming and then material sintering, and also the use of other methods, e.g. an organic matrix and lyophilisation of ceramic slip [47]. The basic bioactive ceramic materials used for scaffolds is calcium phosphate (CaPs), as the main component of bone, and in hydroxyapatite (HA), β-tricalcium phosphate (β-TCP) or a mixture of HA and β-TCP, known as biphasic calcium phosphate [61-63]. A classical solution in the domain of ceramics, are porous scaffolds/corundum implants completely

biocompatible, growing through the fully viable bone tissue, possessing mechanical strength sufficient for many types of clinical procedures and ensuring freedom of manipulation during a surgical procedure, and after growing through, have an appropriate modulus of elasticity, which ensures their good interworking with the bone and also allow for sterilisation with any method. Both, bioactive and biodegradable polymers can be employed [64, 65], including in particular natural polymers such as: collagen, fibrin, alginate, silk, hyaluronic acid and chitosan used, e.g. for bone reconstruction [66], as well as synthetic ones, such as poly(lactic acid) (PLA), poly(glycolic acid) (PGA), and polycaprolactone (PCL) and poly(propylene fumarate) (PPF) with high compressive strength, comparable to this of a cortical layer of bone [65], and some of them, such as poly(lactic acid) (PLA), poly(glycolic acid) (PGA) may cause negative tissue reactions [67]. Composite materials satisfy mechanical and physiological requirements, e.g. CaP-polymer scaffolds, interconnected tricalcium phosphate (TCP) scaffolds coated inside pores with polycaprolactone (PCL) [68], hydroxyapatite HA/poly(ester-urethane) (PU) [69] or a nanocomposite of collagen and Bioglass [70]. Porous metal materials, though not biodegradable, are used for scaffolds, mainly Ti and Ta [71], also after treatment of pores' surface [72] and biodegradable Mg and its alloys [73, 74, 75], including Mg-Ca alloys [76], and have found their application primarily due to relatively high compressive strength and fatigue strength [65, 77]. An innovative approach consists of introducing pure Mg with interconnected porosity onto bearing plates, bolts and networks made by rapid pressure assisted densification methods, such as rapid hot pressing/Spark Plasma Sintering (SPS) [78]. Pure Mg represents an optimum solution due to its biocompatibility, and the manufacturing technology also ensures good mechanical strength and recovery of the bone. In order to reduce the rate of in-vivo corrosion and prevent necrosis and the blocking of blood flow, Mg with Ca, Zn and Mn alloys can be used, well tolerated by a human organism [79, 80], and also coatings adapted to bioresorbable implants [81-84]. In consideration of biocompatibility, reinforcements in magnesium MMCs include usually, notably, HA [85-90], FA [91], calcium polyphosphate [92], and calcium [91]. Third-generation scaffolds not only allow to create a new bone and allow biomineralisation, but are also osteoinductive, and made of CaP, Si-TCP/HA [93], collagen hydrogel [94]. Substitute scaffolds of bones are often administered with medicines, including gentamycin, vancomycin, alendronate, methotrexate and ibuprofen

[95, 96] and with growth factors and transcription factors [64, 97, 98].

The treatment strategy developed these days are **tissue** engineering methods, respectively, scaffold-based vascularised bone tissue engineering (SBV BTE), Vascular Tissue Engineering (VTE) or scaffold-based tissue engineering (SBTE). Promising results are achieved by the application of tissue scaffolds in combination with autologous bone marrow stem cells and growth factors (mainly BMP-2). Tissue engineering, experiencing rapid growth since the mid-90's of the last century, as a field of technical sciences using medical knowledge and materials engineering methods, has been involved in construction and fabrication of scaffolds maintaining the developing tissues, in manipulation of somatic and stem cells, in influencing the tissues growth conditions and their structure and in maintaining the physiochemical conditions of the environment supporting this growth, in order to produce functional substitutes of damaged tissues and entire organs [99, 100]. Tissue engineering provides technical support for regenerative medicine, enabling utilizasation the achievements of life sciences and modern technologies to develop biological materials capable of restoring, maintaining or improving the functions of particular tissues or organs [101]. The concept of "tissue engineering" was introduced in 1985 by Y.C. Fung [102]. The current methods of organ and tissue replacement employ primarily autographs, allografts or metal devices or such made of other engineering materials [103]. Methods are commonly applied in tissue engineering in which threedimensional engineering constructions permit ex vivo tissue transplantation, injection or implantation for the initiation of stem cells regeneration. Opposite to pure therapies in which stem cells are injected directly into peripheral circulation or located in particular tissues, in numerous clinical cases it is necessary to use stem cells carriers for their transport and scaffolds for threedimensional grouping in a particular place of an organism. Research into the use of stem cells in this context has constantly evolved and has considerably intensified in the last decade [103-113]. Obviously, the efficiency of cellbased therapies depends on the preservation of their viability after implantation [114, 115], and this problem is still relevant. One of the main challengers in scaffold transplantation based on cells is the lack of implantation and the related shortage of mass transport of oxygen and nutrients required for the correct functioning and survival of cells in a damaged avascular tissue [116-120], which may lead to ischaemia of tissues and necrosis [121]. The use of scaffolds usually leads to positive results because, as substitutes of an extracellular matrix (ECM), they ensure structural stability for development of tissues and provide an environment of appropriate signals which stimulate cells for proliferation and differentiation as the functional tissue is becoming mature. Scaffolds, apart from ensuring threedimensional geometrical characteristics, must exhibit adequate mechanical properties, enable adhesion of cells and facilitate their development in order to form a threedimensional tissue structure in conditions simulating a natural micro-environment [103, 122]. It is a task of tissue and bone scaffolds to ensure mechanical preservation of living tissues in a three-dimensional structure and ensure an appropriate environment of development for them. Bone scaffolds are usually made of porous biodegradable material, ensuring mechanical support during regeneration of the damaged or injured bone [65, 123]. The role of scaffolds, including also bone scaffolds, is to ensure adhesion and migration of cells and ensure the necessary conditions of their growth by promoting the growth of new blood vessels [65, 124-126], serving to deliver organic substances and diffusion of nutrients and other necessary substances, as well as to ensure appropriate mechanical and physiochemical properties supporting tissue integration and development. Valuable research into the selection of materials for scaffolds is also purused in Poland [122, 127-136]. The general criteria of materials selection for tissue scaffolds relate to material type and its structure, ability to osteoconductivity, mechanical strength, ease of production and manipulation in clinical applications. A microscopic, porous structure of scaffolds is required, enabling diffusion of nutrients and metabolism products by them. The sizes of pores should be adapted to the specific cell type and be large enough to enable migration of cells and creation of an extracellular matrix (ECM), the supply of developmental signals to cells and the promotion of cells acquisition from the surrounding tissues, and small enough to prevent the sealing of pores in a scaffold [103]. It is necessary to ensure conditions to fill up scaffold pores by the reconstructed cells and to guarantee neovascularisation [137] for preventing blood clots [138]. Regeneration in a natural condition forces the removal of an artificial scaffold [139], most advantageously through bioabsorption, which is ensured by numerous natural and synthetic substances used for creation of scaffolds [140, 141]. The rate of bioabsorption should correspond to the rate of the given tissue's regeneration which allows, in particular, to gradually accept a mechanical load by the tissue.

Among others, **cell therapies**, which in case of many disorders enjoy an unrivalled position, have become attractive along with the advancement of tissue engineering

and regenerative medicine. Autologous cells (obtained directly from an organism of the future recipient), isogenic (syngeneic) cells (coming from organisms with an identical genetic material: monozygotic twins, clones, animal lines subject to inbreeding for long time), allogeneic cells (coming from a donor of the same species, e.g. fibroblasts from connective tissue of the prepuce, for producing skin transplants), xenogenic (obtained from other living organisms) represent a source of cells for tissue engineering [142]. They can be primary cells at the same time (coming directly from a living organism) or secondary cells (taken from the cells and tissues bank). Stem cells (cells from the stem) used, e.g. for craniofacial reconstruction [143-150], are characteristic for their lack of differentiation and ability to the unlimited number of divisions in order to obtain more highly specialised cells which, depending on the source, are classified as germ cells (obtained from an embryo) or somatic cells (coming from an adult organism), although the both categories can be crossed by embryonic cloning and by somatic-cell nuclear transfer (SCNT) [151], also in combination with the use of biodegradable scaffolds [152]. Autologous stem cells are the ones most beneficial as they do not cause an immunological response and thus do not cause harmful immunosuppressive side effects. Depending on the tissue development stage, stem cells can be divided into the category of adult and stem embryotic cells [145-147]. Autologous stem cells and progenitor cells may come from umbilical cord blood [153] or tissue [154]. Adult stem cells occur, in particular, in bone marrow, peripheral blood, fatty tissue, nervous tissue, muscles and dermis, and have an ability of transformation into multiple tissues, including bones, gristle, muscles, tendons. Stem cells originating from bone marrow and fatty tissue may be used for breeding mesenchymal cells and tissues, in adipocytes, chondrocytes, osteoblasts and skeletal myocytes and can be used for producing tissues, e.g. fat, gristle, bones and muscles [155-158]. Stem cells originating from bone marrow exhibit a large potential for autologous therapies [147], without immunosuppresive treatment [159-161]. Differentiated cells forming structures of an adult organism represent a more difficult material for breeding. The development of breeding techniques of human stem cells leads to the introduction of the next, new clinical regenerative procedures having no competition in other clinical methods used to date, including treatment of cancer, injuries, inflammation or diseases related to advanced age, and potentially even in treatment of Parkinson's disease and Alzheimer's disease, osteoporosis and heart and liver diseases, metabolic coronary diseases

and autoimmune disorders [103]. It is nevertheless thought that, compared to embryonic stem cells, adult stem cells are usually useful to a limited extent for restoration of different types of cells and tissues [103].

The traditional, and also the oldest fabrication technologies of scaffolds with porous structure differentiate the method of emulsifying/lyophilisation [162], to Thermally Induced Phase Separation (TIPS) [163], Solvent Casting & Particulate Leaching (SCPL), where solvent residues may have an adverse effect on cellular structures [164]. The use of the aforementioned classical methods has not been abandoned altogether, despite being unable to control accurately the size, shape, distribution and interconnections of pores, as well as a general shape of the scaffold. It is used as a modern method in tissue engineering replication technologies with micro/nano patterned surfaces [165-167]. The **master moulds**, for the reason of mould rigidity, are produced using a hard or a soft material. Synthetic and natural biodegradable polymers can be cast onto micro/ nanofabricated moulds to produce structures with small feature resolution [168, 169], including hot embossing (also known as nanoimprint lithography) and soft lithography (micro-casting) for achieving patterns with dimensions about of 5 nm [170-173].

The methods currently in use do not require moulds (solid freeform fabrication SFF) for fabrication of scaffolds made of different materials, including polymer materials, hydrogels, ceramic materials and metallic materials [50, 65, 174-176]. The key tasks in this field include wide application of the particular fabrication methods, not only for the mentioned biocompatible engineering materials, but also for the processing of biological materials [113]. In the three-dimensional printing method (3DP) [177], the particular layers of powder are sprayed with an adequate biocompatible binding agent, e.g. for merging powder to fabricate scaffold from collagen [178], and a 25% acrylic acid solution in a mixture of water with glycerine [179] is used for the integration of hydroxyapatite used for bone regeneration and an aqueous citric acid solution is used for integration of ceramics based on calcium phosphate [180]. A replica of the scaffold surface, e.g. for manufacturing bone and gristle substitutes, can be fabricated with the SFF method of three-dimensional printing hot wax droplets [181]. The limitations of the method originate from wax impurities with biologically incompatible solvents [182], which is not exhibited by new generation materials such as BioBuild and BioSupport dissolving in ethanol or water [182]. The stereolithography method permits to shapen threedimensional form of liquid polymer [183], in particular

using poly(propylene fumarate) (PPF) [184, 185], poly-(ethylene glycol) (PEG) [186, 187]. Polymer materials without solvents, including poly(e-caprolactone) PCL [188, 189], poly(ethylene glycol)-poly(\varepsilon-caprolactone)poly(lactide), PEG-PCL-PLA [189, 190] acrylonitrilebutadiene-styrene (ABS) [191] and hydroxyapatite-poly(εcaprolactone) HA-PCL [189, 192] are used in Fused **Deposition Modelling (FDM)** [193]. The particular layers are placed from a computer controller and using Computer Aided Design (CAD) methods. Selective Laser Sintering (SLS) is similar to 3D printing starting with uniform spreading of a thin layer of powder onto the surface and then the merging of powder grains as a result of sintering with the neighbouring grains with partial pre-melting, according to the assumed constructional characteristics of the element produced, in particular a scaffold, using a computer controlled laser beam according to CAD software. The next layers are manufactured subsequently according to the same method, until the full dimensions of the manufactured element are achieved. This technique, used commonly for additive manufacturing from metallic and ceramic materials [131, 194], including, notably, implants for dental purposes [46], was utilised for scaffolds preparation [50] from biodegradable polymers, e.g. polyether polymer, poly(vinyl alcohol), polycaprolactone [195] and poly(L-lactic acid) [196], and also hydroxyapatite [197] and from composites composed of some of such polymers and hydroxyapatite [196, 198, 199].

Nanofibrous scaffolds are manufactured by electro**spinning**, and the so obtained nanofibres with the diameter of 5 nm to over 1 mm are continuous and randomly interconnected [200, 201]. Due to the character of electrospinning, fibres are oriented randomly [202] or are arranged in an orderly manner [203], they exhibit their structure similar to the extracellular matrix (ECM), have a large specific surface area, high porosity, small size of pores and small density [204]. Natural and engineering materials can be used as a material, including, in particular, collagen, gelatine, chitosan [200]. The ability of certain biopolymers, such as peptides and nucleic acids, to selforganisation, consisting of non-covalent interactions for spontaneous fabrication of a three-dimensional structure in response to the activity of environmental factors [205-207] is utilised for scaffolds fabrication. Such types of scaffolds were used, e.g. for regeneration of nervous tissue to stop bleeding and repair infarcted myocardia, as well as in medical products for slow release of a medicine [208, 209] and for DNA, where the branched DNA particles hybrydise with each other in the presence of ligases in hydrogel [210]. The scaffold fabrication method employing self-

organisable nanofibres is one of few allowing to produce biocomponents with their properties similar to the natural extracellular matrix (ECM), and scaffolds containing hydrogel, made using such technology, employ more advantageous toxicological properties and higher biocompatibility than traditional materials. Conventional hydrogels are particularly useful for three-dimensional placement of cells [211]. Hydrogels used in tissue engineering should have low viscosity before injection and should be gelling fast in the physiological environment of the tissue, and the most important is gelling (sol-gel transition) by crosslinking, which may take place when producing them in vitro and in vivo during injection. Physical cross-linking is used in particular in the case of Poly(N-isopropylacrylamide) (poly(NIPAAM)), which may be used in tissue engineering after introducing acrylic acid (AAc) or PEG [212, 213] or biodegradable polymers, including such as chitosan, gelation, hyaluronic acid and dextran [214-218] to block copolymers, such as poly(ethylene oxide) PEO-PPO-PEO (Pluronic), poly(lactide-co-glycolide) PLGA-PEG-PLGA, PEG-PLLA-PEG, polycaprolactone PCL-PEG-PCL and PEG-PCL-PEG [219-223], and also agarose (a polysaccharide polymer material, extracted from seaweed as one of two principal components of agar) [211], as thermo-sensitive systems [224], to avoid the use of potentially cytotoxic ultraviolet radiation. Poly(NIPAAM) and block copolymer hydrogels may undergo cross-linking as a consequence of temperature and pH acting at the same time, as in the case of acrylates [225, 226], such as 2-(dimethylamino) ethyl methacrylate (DMAEMA) or 2-(diethylaminoethyl) methyl methacrylate. Self-assembling peptides hydrogels, including such containing peptide amphiphiles (PAs), can form nonofibres [227, 228] used for three-dimensional formation of tissue cultures [227, 229-232]. Chemical cross-linking hydrogels having convalescent bonds include photo-crosslinkable poly(ethylene glycol)-diacrylate (PEGDA), poly(ethylene glycol)dimethacrylate (PEGDMA), poly(propylene fumarate) (PPF) and oligo(poly(ethylene glyco) fumarate) (OPF) [233-237], and also natural hydrogels such as dextran, alginate, chitosan and hyaluronic acid synthesised from PEGDA/PEGDMA [238-241] and Michael-type addition reaction [242-244] and Schiff base - crosslinked hydrogels [216, 245-247]. In the case of enzyme-mediated cross-linking [210], transglutaminases (including Factor XIIIa) and horseradish peroxidases (HRP) [211] are used for the catalysis of star-shaped PEG hydrogels [248] and tissue transglutaminase catalysed PEG hydrogels [249] and also tyrosinase, phosphopantetheinyl transferase, lysyl oxidase, plasma amine oxidase, and phosphatases [250],

which in particular have enabled to develop new gels by engrafting tyramine groups into natural and synthetic polymers such as dextran, hyaluronic acid, alginate, cellulose, gelatin, heparin and PEG-PPO [251-257]. Ionic crosslinking hydrogels include calcium-crosslinked alginate [211] and chitosan–polylysine, chitosan–glycerol phosphate salt and chitosan-alginate hydrogels [258-260]. Different synthetic and natural polymers were used for this purpose, including polyethylene glycol (PEG), and copolymers containing PEG [261], hyaluronic acid (HA) [241, 262] after an oxidation reaction through HA-tyramine conjugates [251] and as a result of formation between HA-SH [242, 263] and Michael addition [243, 264], collagen and gelatin hydrogels mostly cross-linked using gluteraldehyde, genipin or water-soluble carbodiimides [265-267], chitosan [268-271], dextran 192 [272, 273] and alginate [274]. Hydrogels were used for reconstruction of the retina [275], ligament [276], fatty tissue [216], kidneys [277], muscles [278], blood vessels [279, 280], and also heart, neural cells, invertebral discs, bones and gristle [211]. Hydrogels were used to prevent adhesions [281, 282], to promote cellular adhesion [244, 283, 284]. So-called strong hydrogels were developed to improve mechanical properties [285]. Threedimensional representation is possible of placement of cells with energy in hydrogel to vascular structures using a laser [286, 287], notably for recording directly the endothelial cell [287]. The most technologically advanced methods of three-dimension printing include at present direct organ **printing** [288, 289], ensuring the highest currently possible degree of control over the structure of the regenerated tissues. Many layers of different types of cells can be printed to create an organ [290]. A polymer-cell mixture can be dosed using this technique, leading to formation of cell hydrogel [291], microfluidics allows for the creation of three-dimensions systems of cells [292], and hydrogels from photopolymerisation polymer solutions can also be used [293], and also SFF techniques, including stereolithography techniques to create scaffolds made of PEG hydrogels [187]. The first production system for threedimensional printing of tissues was delivered only in 2009 based on the NovoGen bioprinting technology [294]. A three-dimensional structure is obtained by subsequent formation of layers of living tissues on the gel or sugar matrix substrate [295].

Unfortunately, despite immense progress in the production of complicated tissue structures in the last several years, the progress in **vascularisation** control is limited. Vascularisation, even for organ printing, still remains a big challenge in tissue engineering. The development of a vascular network in metabolically functional tissues

enables the transport of nutrients and removal of wastes, ensuring maintenance of cells' viability for long time [136]. Micro-formation techniques, by the three-dimensional printing of templates made of agarose fibres, are used for creation of a micro-channel network inside hydrogel products, including, in particular, inside methacrylated gelatin (GelMA), star poly(ethylene glycol-co-lactide) acrylate (SPELA), poly(ethylene glycol) dimethacrylate (PEGDMA) and poly(ethylene glycol) diacrylate (PEGDA) with different concentrations. The efficient formation of endothelial monolayers within the fabricated channels has also been confirmed [296]. Press reports announce, on the other hand, that China has invested nearly 0.5 billion USD to establish 10 national institutes for development of organ printing [297], in which the printing of ears, liver and kidneys from living tissues was started in 2013 and it is expected that fully functional printed organs can be achieved over the next dozens years or so [298, 299]. In the meanwhile, there were reports in the first weeks of the second quarter of this year that an Australian team obtained a kidney tissue print with this method for the first time [300], and an American team confirmed on 1 August 2014 it is ready to print a heart [301].

3. The actual development results of the global markets of biomaterials and various medical products

The existing **global medical products market** is split into numerous segments. In the next part of the paper selected information on the few most important segments of the global markets of biomaterials and various medical products are presented.

The undertaken foresight research shows that the **global** market of Medical Bionic Implants (Artificial Organs), as defined above, will grow in 2012-2017 by 7.1% (with the expected compound annual growth rate (CAGR)), reaching the value of USD 17.82 billion in 2017 [302], and the market of tissue engineering and regenerative medicine will grow in the USA from only USD 6.9 billion in 2009 to USD 32 billion in 2018 [51]. This constitutes a realistic and tangible reason for the intensification of research and implementation works combining activities, notably, in scope of pharmacy, bioengineering, biotechnology, chemistry, electronics and biophysics, which inevitably leads to higher industrial expenditures for investments associated with the acquisition of know-how and expansion of manufacturing capacities in this field.

A market potential analysis indicates clear development tendencies of global markets relating to the paper's subject, although none of them corresponds to this topic directly. From among the **global medical product markets**, directly relevant in connection with the subject of the paper are, most of all, development tendencies of the biomaterials market, medical bionic implant/artificial organs market, orthopaedic devices market, orthopaedic soft tissue repair

market, orthopaedic trauma fixation devices market, orthopaedic soft tissue repair market, and 3D Printing in Medical Applications Market. The topics included in the paper's content are supplementary to such markets.

The comparison of the selected segments of the global markets of biomaterials and various medical products is presented in the Table 1.

Table 1. Examples of the selected segments of the global markets of biomaterials and various medical products

The selected segments of the global markets	The expected compound annual growth rate (CAGR) %	The value of global market USD	The estimated value of global market USD	The source
Global biomaterials market	2013-2019 4.1	2012 25,277.8 million	2019 33,600 million	[2]
Global market of Medical Bionic Implants (Artificial Organs)	2012-2017 7.1	2012 12.67 billion	2017 17.82 billion	[303]
Global orthopaedic devices market	2013-2019 4.9	2012 29.2 billion	2019 41.2 billion	[3]
Global orthopaedic trauma fixation devices market	2014-2019 7.2	2014 6.1 billion	2020 9.3 billion	[304]
Global orthopaedic soft tissue repair market	2013-2019 7.2	2013 5.6 billion	2019 8.5 billion	[305]
3D Printing in Medical Applications Market	2013-2019 15.4	2012 354.5 million	2019 965.5 million	[306]

The **global biomaterials market** was valued at USD 25,277.8 million in 2012 and is expected to grow at a CAGR of 4.1% from 2013 to 2019, to reach an estimated value of USD 33,600 million by 2019 [2]. A generic structure of the global biomaterials market valued at USD billion was shown according to KOL Opinions, Company Annual Reports, Expert Interviews, Investing Publications, Press Releases & TMR Analysis, as well as the global orthopaedic devices market. Biomaterials are used to treat effectively various diseases, such as, in particular, bone cancer, orthopaedic injuries, tissue damages, cardiovascular diseases, dental diseases. Biomaterials are biocompatible and do not cause any immunological reactions in a human organism. The dramatic growth of the market and usage of implants has been seen in developed countries such as the

United States, Canada, Germany, France, Great Britain, Italy and Spain, due to a high utilisation rate of medical implantology procedures as compared to weaker growth elsewhere in the world. North America is the biggest market of biomaterials, lying ahead of Europe. Demand for numerous medical implants and implantation procedures across the world has been rising due to aging population, and longer life expectancy – due to improved healthcare standards – leads to a high incidence rate of arthritis and osteoporosis. The incidence of bone diseases and fractures is more and more common. Orthopaedic applications enjoyed a large share in the global biomaterials market in 2012 due to the growing number of implanted hip and knee joint endoprosthesis. The studied circumstances are closely linked also to the scaffolds with orthopaedic and

craniofacial implants. Society aging has also a great effect on the incidence of eye diseases and dental problems also covered in the paper. Safe, reliable and affordable biomaterials include metals, ceramics, polymers and biomaterials of natural origin. All of the materials are listed within the scope of the multi-aspect focus of the paper. Metallic materials had the largest share in the global biomaterials market in 2012, with a rapidly growing portion of polymer biomaterials. It is estimated that the share of polymers will grow fastest between 2013 and 2019, including nanofibres made of biodegradable polymers as skin and soft tissue scaffolds. Polymers are used in many prostheses such as percutaneous transluminal coronary angioplasty (PTCA) catheters, heart valves, contact lenses, intraocular lenses and for constructing rigid bases for dental prosthesis and dentures, in ophthalmic applications, and in urology and gastroenterology, and to an artificial esophagus. North America and Europe maintain their leading position on the global biomaterials market for the entire projected period of 2013 to 2019, but countries of Asia and Pacific, such as Japan, South Korea, China, India and Taiwan play more and more crucial part in biomaterials market development, and development will also be seen in Latin America in the vears to come.

The medical bionic implant and artificial organs market is a potentially growing one with a global market of \$12.67 billion in 2012 as it is expected to grow at a CAGR of 7.1% to reach \$17.82 billion in 2017 [303]. The development trend of the medical bionic implant and artificial organs industry has maintained over the past two decades and it is expected that will continue until the 20's. The global medical bionic implant and artificial organs market has been segmented into five categories based on the type of products, technology used, and type of fixation, including vision bionics, ear bionics, orthopaedic bionics, heart bionics, and neural/brain bionics. New and improved technologies, increasing organ failure owing to aging and age-related disorders, increasing accidents and injuries leading to amputations, and rise in number of people awaiting organ transplants are the major drivers slated to propel the growth of this market. North America dominates the artificial organs market in 2012, followed by Europe.

The **global orthopaedic devices market** was valued at USD 29.2 billion in 2012 and is expected to grow at a CAGR of 4.9% from 2013 to 2019, to reach an estimated value of USD 41.2 billion in 2019 [3]. Orthopaedic devices are used to restore skeletal structure and joint movements in various types of fractures, abnormal growth of bones, soft tissue damage, trauma or other deformities. These

devices can be surgically implanted or externally attached through minimally invasive procedures and hence can be classified as joint implants, internal and external fixation devices. Demand for orthopaedic procedures is expected to grow in the near future owing to the increase in geriatric population and obesity across the globe. The major orthopaedic device segments such as joint implants, internal and external fixation devices have been further analysed on the basis of anatomical locations namely, hip, knee, shoulder, elbow, foot and ankle and other extremities. Spinal orthopaedic devices have been segmented into joint implants and internal fixation devices, while the craniomaxillofacial devices market include estimations only for internal fixation devices.

The global orthopaedic trauma fixation devices market is estimated at USD 6.1 billion in 2014 and is expected to grow at a CAGR of 7.2% from 2014 to 2019, to reach an estimated value of USD 9.3 billion in 2020 [304]. The key market drivers include rising healthcare spendings, popularisation of sports activity, a growing number of road accidents and growing geriatric population, leading to higher number of fractures and injuries. The impediments for development are high treatment costs, poor knowledge among many people and disregarding such type of disorders in healthcare systems, especially in developing countries. Internal fixators have the largest share in the orthopaedic trauma fixation devices market and are projected to grow at a CAGR of 6.8% until 2020. Plate and screw systems are used most often and their development in this period will be 7.1%, and internal fixators are used more and more often with bioabsorbable material and development of their production will be even higher and will be 8.4%. North America, including the U.S., has the largest orthopaedic trauma fixation devices market, while Asia, especially China, Japan and other Southeast Asia countries and also countries of the eastern Mediterranean countries are growth markets.

The global orthopaedic soft tissue repair market was valued at USD 5.6 billion in 2013 and is expected to grow at a CAGR of 7.2% from 2013 to 2019, to reach an estimated value of USD 8.5 billion in 2019 [305]. The key market development drivers include society aging, increase in obesity, a higher number of damaged soft tissues, including largely due to sports injuries, and also introduction of new medical technologies, and no other alternatives to repair soft tissues, apart from surgical ones, and also growing healthcare expenditures. The constraints encountered by the market are associated especially with a tendency of forcing out metal implants by biodegradable materials, which requires a technology change and usage of

robot-assisted surgeries at the expense of traditional surgical methods related to growth of costs. ACL/PCL reconstruction is the largest practiced procedure in the orthopaedic soft tissue repair market and it is expected to grow at a CAGR of about 8.3% during 2013-2019. Other widely used orthopaedic soft tissue repair procedures include Meniscal Repair, Hip Arthroscopy, Rotator Cuff, Shoulder Labrum and Biceps Tenodesis. North America, including the USA, has the largest share in the soft tissue repair market, whilst Asia, China, India and Japan witness the fastest global growth.

The **3D Printing in Medical Applications Market** was valued at USD 354.5 million in 2012. Its growth is estimated at a high CAGR of 15.4% from 2013 to 2019, to USD 965,500,000 [306]. 3D printing technologies have delivered multiple solutions in the medical industry and have revolutionised the healthcare segment by facilitating the manufacturing of medical implants and surgical guides such as dental, orthopaedic and cranio-maxillofacial ones, usually with enhanced efficiency. Fabrication takes place with various materials, such as metals, polymers, ceramics and natural biological cells. New technologies evolve, such as laser beam melting (LBM), electron beam melting (EBM), droplet deposition manufacturing (DDM) and photopolymerisation. The North America region was the biggest 3D printing market for medical applications in 2012, while it is estimated that Europe enjoys the highest growth rate by over 15% between 2013 and 2019.

The analysis made clearly shows a clear development trend of all the world markets of biomaterials and various medical products, with division into traditional sectors of such a market, though. The facts described above substantiate the determination the state of knowledge in this area, which will be the basis for new lines of research and to increase the level of knowledge among engineers and medical doctors.

4. The estimated future research of the hybrid technologies of bioactive and engineering materials for personalised scaffolds of tissues and bones

The development of new **hybrid technologies of bioactive and engineering materials for personalised scaffolds of tissues and bones** requires a number of basic research and application work. These include generally, among others:

- analysing clinical cases in the field of maxillo-facial surgery, restorative dentistry, laryngology, orthopaedics and traumatology, oesophagus and blood vessels prosthetics, for an inventory and classification of typical cases of the necessity to personalise hybrid scaffolds of tissues and bones,
- designing and constructing of the new generations of implants using the currently available methods of advanced medical imaging and simulation of mechanical loads with methods of numerical approximation and Computational Materials Science (CMS) and engineering material, constructional and technological design - Computer Aided Materials Design/Design/Manufacturing CAMD/CAD/CAM and experimental verification of models and calculations in laboratory conditions,
- introducing the bioactive and engineering materials for above applications and investigating the structure and properties of the examined materials subject to the applied technological processes, among others using advanced methods of light and confocal microscopy, scanning probes, transmission and scanning methods including HRTEM, spectral methods EDS, WDS, EBSD, GDOS, FTIR, Raman's method, X-ray structure analysis, dilatation investigations, mechanical investigations, including micro- and nano-hardness, investigations of physiochemical, corrosive and tribological properties,
- biological and biocompatibility investigations, cytotoxic investigations, investigations of biotrans- formation mechanisms and processes using immonu- cytochemistry, immunofluorescence and molecular biology techniques,
- preparatory works for implementation in industrial conditions at the semi-technical scale, including market research for the prospect product, preparation of technical documentation necessary for implementation, preparation of procedures related to the market use of a future product originating from the research, obtaining a certificate of conformity entitling to mark a product with a mark for conformity to national or foreign standards, certification and actions directly related to procedures for granting the rights.

The following Table 2 presents numerous examples of the application of various bioactive and engineering materials, and their respective materials processing and tissue engineering technologies for manufacturing of the hybrid personalised implants and scaffolds.

Table 2. Examples of the application of various bioactive and engineering materials, and their respective materials processing and tissue engineering technologies for manufacturing of the hybrid personalised implants and scaffolds

Fabrication stage	Investigated materials	Technologies applied	Areas of application
Fabrication of implant bearing structure	Ti, Ti alloys with V or Nb, Mg (possibly with additives of Ca, Zn and Mn), ceramic materials Al ₂ O ₃ and ZrO ₂ , TiO ₂ , resorbable bioglass, e.g. Hench bioglass, from the CaO-SiO ₂ -P ₂ O ₅ and SiO ₂ -Al ₂ O ₃ system, hydroxyapatites, polymers, composites	Selective Laser Sintering, sintering, the use of organic matrix, lyophilisation of ceramic slip, rapid pressure assisted densification methods, such as rapid hot pressing/Spark Plasma Sintering (SPS), sheletal posting plactic working outling	
Fabrication of implant porous part	Ti, Ti alloys with V or Nb, Mg (possibly with additives of Ca, Zn and Mn), ceramic materials Al ₂ O ₃ and ZrO ₂ , TiO ₂ , resorbable bioglass, e.g. Hench bioglass, from the CaO-SiO ₂ -P ₂ O ₅ i SiO ₂ -Al ₂ O ₃ system, hydroxyapatites, polymers, composites	facturing, sol-gel methods, 3D printing, sol-gel methods, 3D print	
Fabrication of coatings inside pores of implant porous part	natural protein, synthetic and polysaccharide polymers, including thermosetting, including collagen, fibrin, alginate, silk, hyaluronic acid, chitosan, poly(lactic acid) (PLA), poly(glycolic acid) (PGA), polycaprolactone (PCL) and poly(propylene fumarate) (PPF), polyethylene glycol, Al ₂ O ₃ , resorbable bioglass, hydroxy carbonate apatite (HCA), calcium phosphate (CaPs), hydroxyapatite (HA), β-tricalcium phosphate (β-TCP), biphasic calcium phosphate, composites: collagen + hydroxyapatite CaP-polymer tricalcium phosphate (TCP)-polycaprolactone (PCL), hydroxyapatite HA/poly(ester-urethane)(PU), collagen-Bioglass	Inflirtation, 3D printing, selective laser sintering, electrospinning, atomic layer deposition, Physical Vapour Deposition, pressing, sol-gel methods	and knee joints, facial-skull bone, losses of joint cartilage cells, oesophagus losses and/or blood vessel losses, dental restorations, skin restorations
Fabrication and application of tissue cultures	adipocytes, chondrocytes, osteoblasts, fibroblasts and skeletal myocytes	Cell transplantation, matrix implantation, cell implantation with matrix, breeding of xenogeneic and autologous cells and the stage of clinical activities	

5. General conclusion

A thorough undertaken state-of-the-art shows the high technological advancement of tissue engineering methods. The high advancement of prosthetics/implantation techniques used in the clinical practice should also be noted, which is not detailed in this description as the issues are commonly known. The positioning and fixing of implants takes place in all those methods in a classical way

using mechanical devices and solutions. There are no reports in the references about an original concept presented by the Author of introduction of prosthetics/implantation and tissue engineering techniques for the purpose of natural ingrowth of the implanted elements into a living tissue in the implant area without having to use mechanical devices, at least in the connection (interface) zone of bone or organ stumps with prosthetic/implant elements. This opens up vast possibilities for the application of the hybrid technologies of bioactive and

engineering materials for personalized scaffolds of tissues and bones in accordance with the concept of the Author, presented in this paper.

References

- [1] A. Arsiwala, P. Desai, V. Patravale, Recent advances in micro/nanoscale biomedical implants, Journal of Controlled Release 189 (2014) 25-45.
- [2] Biomaterials Market for Implantable Devices (Material Type - Metals, Polymers, Ceramics and Natural, Applications - Cardiology, Orthopedics, Dental, Ophthalmology and Others) - Global Industry Analysis, Size, Share, Growth, Trends and Forecast, 2013 - 2019, Transparency Market Research, 2014, http://www.transparencymarketresearch.com/biomateri als-market.html.
- [3] Orthopedic Devices Market (Hip, Knee, Spine, Shoulder, Elbow, Foot and Ankle, Craniomaxillofacial and Other Extremities) Global Industry Analysis, Size, Share, Growth, Trends and Forecast, 2013 2019, Transparency Market Research, 2014, http://www.transparencymarketresearch.com/orthopedic-devices-market.html.
- [4] Health and Health Care in 2012, GUS, Warsaw 2012.
- [5] Statistical Yearbook of the Republic of Poland 2013, GUS, Warsaw 2014.
- [6] L.A. Dobrzański et al., Development of a new composite material with a gradient of the polymer matrix reinforced with aramid fibers and titanium powder particles, for the production of esophageal prosthesis intrasystemic, Project N507 422136, Gliwice 2009-2011.
- [7] L.A. Dobrzański, Report on the main areas of the materials science and surface engineering own research, Journal of Achievements in Materials and Manufacturing Engineering 49/2 (2011) 514-549.
- [8] L.A. Dobrzański et al., Establishing a methodology of computer-aided material, technological and construction design of fixed dental multi-component prostheses for predicting their functional properties, Project N507 438539, Gliwice 2010-2013.
- [9] L.A. Dobrzański et al., Determining the importance of the effect of the onedimensional nanostructural materials on the structure and properties of newly developed functional nanocomposite and nanoporous materials, Project UMO-2012/07/B/ST8/04070, Gliwice 2013.
- [10] L.A. Dobrzański, Descriptive metal science, Publishing House of the Silesian University of Technology, Gliwice, 2013 (in Polish).

- [11] L.A. Dobrzański et al., Investigations of structure and properties of newly created porous biomimetic materials fabricated by selective laser sintering, Project UMO-2013/08/M/ST8/00818, Gliwice 2013.
- [12] L.A. Dobrzański et al., Foresight of surface properties formation leading technologies of engineering materials and biomaterials. Project UDA-POIG.01.01.01-00.23/08-00, Gliwice 2009-2012.
- [13] L.A. Dobrzański, M. Pawlyta, A. Hudecki, Conceptual study on a new generation of the high-innovative advanced porous and composite nanostructural functional materials with nanofibers, Journal of Achievements in Materials and Manufacturing Engineering 49/2 (2011) 550-565.
- [14] L.A. Dobrzański, A.J. Nowak, W. Błażejewski, R. Rybczyński, The concept of preparation of oesophageal prosthesis based on long-fiber composite material. Journal of Achievements in Materials and Manufacturing Engineering 46/1 (2011) 18-24.
- [15] L.A. Dobrzański, M. Hetmańczyk, E. Łagiewka, Current state and development perspectives of Materials Science and Engineering in Poland, Journal of Achievements in Materials and Manufacturing Engineering 43, 782-789;
- [16] K. Cholewa-Kowalska, J. Kokoszka, M. Łączka, Ł. Niedźwiedzki, W. Madej, A.M. Osyczka, Gel derived bioglass as a compound of hydroxyapatite composites. Biomedical Materials 4 (2009) 055007.
- [17] P. Konieczny, A.G. Goralczyk, R. Szmyd, L. Skalniak, J. Koziel, F.L. Filon, M. Crosera, A. Cierniak, E.K. Zuba-Surma, J. Borowczyk, E. Laczna, J. Drukala, E. Pyza, D. Semik, O. Woznicka, A. Klein, J. Jura, Effects triggered by platinum nanoparticles on primary keratinocytes, International Journal of Nanomedicine 8/1 (2013) 3963-3975.
- [18] M. Kozdęba, J. Borowczyk, E. Zimolag, D. Dziga, M. Wasylewski, Z. Madeja, J. Drukala, Microcystin-LR affects properties of human epidermal skin cells crucial for regenerative processes, Toxicon 80 (2014) 38-46.
- [19] R. Major, F. Bruckert, J.M. Lackner, J. Marczak, B. Major, Surface treatment of thin-film materials to allow dialogue between endothelial and smooth muscle cells and the effective inhibition of platelet activation. The Royal Society of Chemistry: Advances 4 (2014) 9491-9502.
- [20] A. Mzyk, R. Major, M. Kot, J. Gostek, P. Wilczek, B. Major, Chemical control of polyelectrolyte film properties for an effective cardiovascular implants endothelialization, Archives of Civil and Mechanical Engineering 14/2 (2014) 262-268.

- [21] B. Major et al., CardioBioMat Nanostructural materials for biomedical cardiovascular systems, International Project ERA-NET MNT, 2009-2012.
- [22] P. Tomasik, J. Spindel, L. Miszczyk, A. Chrobok, B. Koczy, J. Widuchowski, T. Mrozek, J. Matysiakiewicz, B. Pilecki Treatment and differential diagnosis of aneurysmal bone cyst based on our own experience, Ortopedia Traumatologia Rehabilitacja 11/5 (2009) 467-475
- [23] A.B. Ostałowska, S. Kasperczyk, A. Kasperczyk, L. Słowińska, M. Marzec, T. Stołtny, B. Koczy, E. Birkner, Oxidant and anti-oxidant systems of synovial fluid from patients with knee post-traumatic arthritis, Journal of Orthopaedic Research 25/6 (2007) 804-812.
- [24] T. Stołtny, B. Koczy, W. Wawrzynek, L. Miszczyk, Heterotopic ossification in patients after total hip replacement, Ortopedia Traumatologia Rehabilitacja 9/3 (2007) 264-272.
- [25] T. Mrożek, J. Spindel, L. Miszczyk, B. Koczy, A. Chrobok, B. Pilecki, P. Tomasik, J. Matysiakiewicz, Treatment methods for neoplastic metastates and tumor-like changes in the bodies and epiphyses of long bones using polymethyl methacrylate cement and bone grafting, Ortopedia Traumatologia Rehabilitacja 7/5 (2005) 481-485.
- [26] P. Tomasik, J. Spindel, B. Koczy, A. Chrobok, T. Mrożek, J. Matysiakiewicz, L. Miszczyk, Clinical experience in the application of allogenic grafts from a bone tissue bank in the surgical treatment of tumorlike bone lesions, Ortopedia Traumatologia Rehabilitacja 7/5 (2005) 476-480.
- [27] M. Olakowski, H. Mieczkowska-Palacz, E. Olakowska, P. Lampe, Surgical management of pancreatico-pleural fistulas, Acta Chirurgica Belgica 109/6 (2009) 735-740.
- [28] J. Dec, T.S. Gaździk, H. Bursig, A. Wysocka, J. Jędrysik, H. Noga, Treatment of full thickness knee cartilage defects using Autologous Chondrocyte Implantation, Arthroscopy and Joint Surgery 5/3-4 (2009) 25-26.
- [29] A. Wysocka-Wycisk, F. Kępski, H. Bursig, S. Dyląg, T.S. Gaździk, Autologous chondrocytes culture, The Journal of Orthopaedics Trauma Surgery and Related Research 4/20 (2010) 110-115.
- [30] T.S. Gaździk, A. Wysocka, M. Marek, J. Dec, J. Jędrysik, H. Noga, H. Bursig, S. Dyląg, Further observation on the use of autological chondrocytes in the treatment of demages of knee joint cartilage, The Journal of Orthopaedics Trauma Surgery and Related Research 2/22 (2011) 69-74.
- [31] M.B. Nessler, J.W. Puchała, J.A. Drukała, Changes in me plasma cytokine and growth factor profile are

- associated with impaired healing in paediatric patients treated with INTEGRA® for reconstructive procedures, Burns 39/4 (2013) 667-673.
- [32] L.A. Dobrzański, M. Szczęsna, eds., Laboratory classes in materials science, Open Access Library 12 (2013) 1-215 (in Polish).
- [33] L.A. Dobrzański, T. Tański, eds., Laboratory classes in materials engineering and nanotechnology, Open Access Library 10 (2013) 1-763 (in Polish).
- [34] L.A. Dobrzański, A.D. Dobrzańska-Danikiewicz, Formation of structure and properties of engineering materials, Publishing House of the Silesian University of Technology, Gliwice, 2013 (in Polish).
- [35] A.D. Dobrzańska-Danikiewicz, The Book of Critical Technologies of Surface and Properties Formation of Engineering Materials, Open Access Library 8 (2013) 1-823 (in Polish).
- [36] J. Nowacki, L.A. Dobrzański, F. Gustavo, Intramedullary implants for osteosynthesis of long bones, Open Access Library 11 (2012) 1-150 (in Polish).
- [37] L.A. Dobrzański, A. Achtelik-Franczak, M. Król, Computer aided design in Selective Laser Sintering (SLS) – application in medicine, Journal of Achievements in Materials and Manufacturing Engineering 60/2 (2013) 66-75.
- [38] L.A. Dobrzański, A. Hudecki, Composite nanofibers with bioactive core and antibacterial coating for tissue scaffolds produced by electrospinning, prepared for print.
- [39] A.J. Nowak, L.A. Dobrzański, R. Rybczyński, R. Mech, Finite Element Method application for modelling of internal oesophageal prosthesis, Archives of Materials Science and Engineering 64/2 (2013) 198-204.
- [40] T. Stefański, P. Malara, A. Kloc-Ptaszna, B. Janoszka, L. Postek-Stefańska, K. Tyrpień-Golder, L.A. Dobrzański, Erosive potential of calcium-supplemented citric acid on bovine enamel, Archives of Materials Science and Engineering 64/2 (2013) 175-181.
- [41] J. Żmudzki, G. Chladek, P. Malara, L.A. Dobrzański, M. Zorychta, K. Basa, The simulation of mastication efficiency of the mucous-borne complete dentures, Archives of Materials Science and Engineering 63/2 (2013) 75-86.
- [42] G. Chladek, J. Żmudzki, P. Malara, L.A. Dobrzański, C. Krawczyk, Effect of Influence of introducing silver nanoparticles on tribological characteristics of soft liner, Archives of Materials Science and Engineering 62/1 (2013) 5-14.
- [43] M. Król, L.A. Dobrzański, Ł. Reimann, I. Czaja, Surface quality in selective laser melting of metal

- powders, Archives of Materials Science and Engineering 60/2 (2013) 87-92.
- [44] Ł. Reimann, L.A. Dobrzański, Influence of the casting temperature on dental Co-base alloys properties, Archives of Materials Science and Engineering 60/1 (2013) 5-12.
- [45] L.A. Dobrzański, Ł. Reimann, Digitization procedure of creating 3D model of dental bridgework reconstruction, Journal of Achievements in Materials and Manufacturing Engineering 55/2 (2012) 469-476.
- [46] L.B. Dobrzański, P. Malara, J. Pacyna, Comparative studies of selected engineering materials containing titanium and selective laser sintering technology SLS and computer-aided manufacturing CAD with the recommendation for a clinical use for permanent dentures and dental surgical supplement, 2014, in progress.
- [47] Z. Jaegermann, A. Ślósarczyk, Dense and porous corundum bioceramics in medical applications, University Scientific and Technical Publishing House, Krakow 2007 (in Polish).
- [48] E. Czarnowska, J. Morgiel, M. Ossowski, A. Sowińska, T. Wierzchoń, Microstructure and biocompatibility of titanium oxide produced on a nitrided surface layer under glow discharge conditions, Journal of Nanoscience and Nanotechnology 11/10 (2011) 8917-8923.
- [49] C.K. Chua, M.J.J. Liu, S.M. Chou, Additive Manufacturing-assisted scaffold-based Tissue Engineering. In: Innovative Developments in Virtual and Physical Prototyping, Proceedings of the 5th International Conference on Advanced Research in Virtual and Rapid Prototyping, Leiria, Portugal, 2011, 13-21.
- [50] A. Mazzoli, Selective laser sintering in biomedical engineering, Medical & Biological Engineering & Computing 51/3 (2013) 245-256.
- [51] P. Zorlutuna, N. Annabi, G. Camci-Unal, M. Nikkhah, J.M. Cha, J.W. Nichol, A. Manbachi, H. Bae, S. Chen, A. Khademhosseini, Microfabricated Biomaterials for Engineering 3D Tissues, Advanced Materials 24/14 (2012) 1782-1804.
- [52] S.E. Yang., K.P. Leong, Z.H. Du, C.K. Chua, The design of scaffolds for use in tissue engineering. Part 1. Traditional factors, Tissue Engineering 7/6 (2001) 679-689.
- [53] P.I. Bartolo, C.K. Chua, H.A. Almeida, S.M. Chou, A.S.C. Lim, Biomanufacturing for tissue engineering: Present and future trends, Virtual and Physical Prototyping 4/4 (2009) 203-216.
- [54] J.R. Jones, L.M. Ehrenfried, L.L. Hench, Optimising bioactive glass scaffolds for bone tissue engineering, Biomaterials 27/7 (2006) 964-973.

- [55] L.L. Hench, Ö. Andersson, Bioactive glasses, in: L.L. Hench, J. Wilson, eds., An Introduction to Bioceramics, Word Scientific, 1993, 41-62.
- [56] L. Ciołek, J. Karaś, A. Olszyna, S. Traczyk, New silver-containing bioglasses, Engineering of Biomaterials 11/77-80 (2008) 25-27.
- [57] L. Ciołek, J. Karaś, A. Olszyna, E. Zaczyńska, A. Czarny, B. Żywicka, In vitro studies of cytotoxicity of bioglass containing silver, Engineering of Biomaterials 12/89-91 (2009) 91-93.
- [58] L. Ciołek, J. Karaś, A. Olszyna, E. Zaczyńska, A. Czarny, B. Żywicka, In vitro antibacterial activity of silver-containing bioglasses, Engineering of Biomaterials 13/100-101 (2010) 21-23.
- [59] B.S. Miguel, R. Kriauciunas, S. Tosatti, M. Ehrbar, C. Ghayor, M. Textor, F.E. Weber, Enhanced osteo-blastic activity and bone regeneration using surface-modified porous bioactive glass scaffolds, Journal of Biomedical Materials Research Part A 94A/4 (2010) 1023-1033.
- [60] C. Wu, Y. Zhou, W. Fan, P. Han, J. Chang, J. Yuen, M. Zhang, Y. Xiao, Hypoxia-mimicking mesoporous bioactive glass scaffolds with controllable cobalt ion release for bone tissue engineering, Biomaterials 33/7 (2012) 2076-2085.
- [61] K. Rezwan, Q.Z. Chen, J.J. Blaker, A.R. Boccaccini, Biodegradable and bioactive porous polymer/inorganic composite scaffolds for bone tissue engineering, Biomaterials 27/18 (2006) 3413-3431.
- [62] V. Karageorgiou, D. Kaplan, Porosity of 3D biomaterial scaffolds and osteogenesis, Biomaterials 26/27 (2005) 5474-5491.
- [63] C.E. Wilson, C.A. van Blitterswijk, A.J. Verbout, W.J.A. Dhert, J.D. de Bruijn, Scaffolds with a standardized macro-architecture fabricated from several calcium phosphate ceramics using an indirect rapid prototyping technique, Journal of Materials Science. Materials in Medicine 22/1 (2011) 97-105.
- [64] P. Lichte, H.C. Pape, T. Pufe, P. Kobbe, H. Fischer, Scaffolds for bone healing: Concepts, materials and evidence, Injury 42/6 (2011) 569-573.
- [65] S. Bose, M. Roy, A. Bandyopadhyay, Recent advances in bone tissue engineering scaffolds, Trends in Biotechnology 30/10 (2012) 546-554.
- [66] S.-H. Lee, H. Shin, Matrices and scaffolds for delivery of bioactive molecules in bone and cartilage tissue engineering, Advanced Drug Delivery Reviews 59/4-5 (2007) 339-359.
- [67] H.-Y. Cheung, K.-T. Lau, T.-P. Lu, D. Hui, A critical review on polymer-based bioengineered materials for scaffold development, Composites Part B: Engineering 38/3 (2007) 291-300.

- [68] W. Xue, A. Bandyopadhyay, S. Bose, Polycaprolactone coated porous tricalcium phosphate scaffolds for controlled release of protein for tissue engineering, Journal of Biomedical Materials Research Part B: Applied Biomaterials 91B/2 (2009) 831-838.
- [69] M.W. Laschke, A. Strohe, M.D. Menger, M. Alini, D. Eglin, In vitro and in vivo evaluation of a novel nanosize hydroxyapatite particles/poly(ester-urethane) composite scaffold for bone tissue engineering, Acta Biomaterialia 6/6 (2010) 2020-2027.
- [70] S.S. Banerjee, S. Tarafder, N.M. Davies, A. Bandyopadhyay, S. Bose, Understanding the influence of MgO and SrO binary doping on the mechanical and biological properties of β-TCP ceramics, Acta Biomaterialia 6/10 (2010) 4167-4174.
- [71] V.K. Balla, S. Bodhak, S. Bose, A. Bandyopadhyay, Porous tantalum structures for bone implants: Fabrication, mechanical and in vitro biological properties, Acta Biomaterialia 6/8 (2010) 3349-3359.
- [72] K. Das, V.K. Balla, A. Bandyopadhyay, S. Bose, Surface modification of laser-processed porous titanium for load-bearing implants, Scripta Materialia 59/6 (2008) 822-825.
- [73] F. Witte, H. Ulrich, C. Palm, E. Willbold, Biodegradable magnesium scaffolds: Part II: Periimplant bone remodelling, Journal of Biomedical Materials Research Part A 81A/3 (2007) 757-765.
- [74] X. Zhang, X.-W. Li, J.-G. Li, X.-D. Sun, Preparation and mechanical property of a novel 3D porous magnesium scaffold for bone tissue engineering, Materials Science and Engineering C 42 (2014) 362-367.
- [75] K.F. Farraro, K.E. Kim, S.L.-Y. Woo, J.R. Flowers, M.B. McCullough, Revolutionizing orthopaedic biomaterials: The potential of biodegradable and bioresorbable magnesium-based materials for functional tissue engineering, Journal of Biomechanics 47/9 (2014) 1979-1986.
- [76] R. Nowosielski, A. Gawlas-Mucha, A. Borowski, A. Guwer, Fabrication and properties of magnesium based alloys Mg-Ca, Journal of Achievements in Materials and Manufacturing Engineering 61/2 (2013) 367-374.
- [77] Y. Yun, Z. Dong, N. Lee, Y. Liu, D. Xue, X. Guo, J. Kuhlmann, A. Doepke, H.B. Halsall, W. Heineman, S. Sundaramurthy, M.J. Schulz, Z. Yin, V. Shanov, D. Hurd, P. Nagy, W. Li, C. Fox, Revolutionizing biodegradable metals, Materials Today 12/10 (2009) 22-32.
- [78] L. Jaworska, B. De Benedetti, 2014, private information.
- [79] N.T. Kirkland, N. Birbilis, M.P. Staiger, Assessing the corrosion of biodegradable magnesium implants:

- A critical review of current methodologies and their limitations, Acta Biomaterialia 8/3 (2012) 925-936.
- [80] N. Li, Y. Zheng, Novel Magnesium Alloys Developed for Biomedical Application: A Review, Journal of Materials Science and Technology 29/6 (2013) 489-502.
- [81] G. Wu, J.M. Ibrahim, P.K. Chu, Surface design of biodegradable magnesium alloys A review, Surface & Coatings Technology 233 (2013) 2-12.
- [82] H. Hornberger, S. Virtanen, A.R. Boccaccini, Biomedical coatings on magnesium alloys A review, Acta Biomaterialia 8/7 (2012) 2442-2455.
- [83] M. Yazdimamaghani, M. Razavi, D. Vashaee, L. Tayebi, Development and degradation behavior of magnesium scaffolds coated with polycaprolactone for bone tissue engineering, Materials Letters 132 (2014) 106-110.
- [84] Z. Chen, X. Mao, L. Tan, T. Friis, C. Wu, R. Crawford, Y. Xiao, Osteoimmunomodulatory properties of magnesium scaffolds coated with β-tricalcium phosphate, Biomaterials 35/30 (2014) 8553-8565.
- [85] X.N. Gu, W.R. Zhou, Y.F. Zheng, L.M. Dong, Y.L. Xi, D.L. Chai, Microstructure, mechanical property, bio-corrosion and cytotoxicity evaluations of Mg/HA composites, Materials Science and Engineering C 30/6 (2010) 827-832.
- [86] A.K. Khanra, H.C. Jung, K.S. Hong, K.S. Shin, Comparative property study on extruded Mg–HAP and ZM61–HAP composites, Materials Science & Engineering A 527/23 (2010) 6283-6288.
- [87] A.K. Khanra, H.C. Jung, S.H. Yu, K.S. Hong, K.S. Shin, Microstructure and mechanical properties of Mg-HAP composites, Bulletin of Material Science 33/1 (2010) 43-47.
- [88] D.B. Liu, M.F. Chen, X.W. Wang, Fabrication and corrosion biodegradable properties of the HA/Mg biocomposite, Rare Metal Materials and Engineering 37/12 (2008) 2201-2205.
- [89] F. Witte, F. Feyerabend, P. Maier, J. Fischer, M. Stormer, C. Blawert, W. Dietzel, N. Hort, Biodegradable magnesium–hydroxyapatite metal matrix composites, Biomaterials 28/13 (2007) 2163-2174.
- [90] X.Y. Ye, M.F. Chen, M. Yang, J. Wei, D.B. Liu, In vitro corrosion resistance and cytocompatibility of nano-hydroxyapatite reinforced Mg-Zn-Zr composites, Journal of Materials Science: Materials in Medicine 21 (2010) 1321-1328.
- [91] M. Razavi, M.H. Fathi, M. Meratian, Microstructure, mechanical properties and bio-corrosion evaluation of biodegradable AZ91-FA nanocomposites for biomedical applications, Materials Science and Engineering A 527/26 (2010) 6938-6944.

- [92] A. Feng, Y. Han, The microstructure, mechanical and corrosion properties of calcium polyphosphate reinforced ZK60A magnesium alloy composites, Journal of Alloys and Compounds 504/2 (2010) 585-593.
- [93] A. Papadimitropoulos, M. Mastrogiacomo, F. Peyrin, E. Molinari, V.S. Komlev, F. Rustichelli, R. Cancedda, Kinetics of in vivo bone deposition by bone marrow stromal within a resorbable porous calcium phosphate scaffold: An X-ray computed microtomography study, Biotechnology and Bioengineering 98/1 (2007) 271-281.
- [94] H. Naito, Y. Dohi, W.-H. Zimmermann, T. Tojo, S. Takasawa, T. Eschenhagen, S. Taniguch, The Effect of Mesenchymal Stem Cell Osteoblastic Differentiation on the Mechanical Properties of Engineered Bone-Like Tissue, Tissue Engineering Part A 17/17-18 (2011) 2321-2329.
- [95] S. Bose, S. Tarafder, Calcium phosphate ceramic systems in growth factor and drug delivery for bone tissue engineering: A review, Acta Biomaterialia 8/4 (2012) 1401-1421.
- [96] E. Verron, I. Khairoun, J. Guicheux, J.-M. Bouler, Calcium phosphate biomaterials as bone drug delivery systems: a review, Drug Discovery Today 15/13-14 (2010) 547-552.
- [97] N. Kimelman-Bleich, G. Pelled, Y. Zilberman, I. Kallai, O. Mizrahi, W. Tawackoli, Z. Gazit, D. Gazit, Targeted gene-and-host progenitor cell therapy for nonunion bone fracture repair, Molecular Therapy 19/1 (2010) 53-59.
- [98] M. Keeney, J.J.P. van den Beucken, P.M. van der Kraan, J.A. Jansen, A. Pandit, The ability of a collagen/calcium phosphate scaffold to act as its own vector for gene delivery and to promote bone formation via transfection with VEGF(165), Biomaterials 31/10 (2010) 2893-2902.
- [99] R.P. Lanza, R. Langer, J. Vacanti, eds., Principles of Tissue Engineering, Academic Press, San Diego 2000.
- [100] A. Atala, R.P. Lanza, eds., Methods of Tissue Engineering, Academic Press, San Diego 2002.
- [101] R. Langer, J.P. Vacanti, Tissue engineering. Science 260/5110 (1993) 920-926.
- [102] Y.C. Fung, A Proposal to the National Science Foundation for An Engineering Research Center at UCSD. Center for the Engineering of Living Tissues, UCSD #865023, 2001.
- [103] F. Yang, W.L. Neeley, M.J. Moore, J.M. Karp, A. Shukla, R. Langer, Tissue Engineering: The Therapeutic Strategy of the Twenty-First Century, in: C.T. Laurencin, L.S. Nair, eds., Nanotechnology and

- Tissue Engineering: The Scaffold, CRC Press Taylor & Francis Group, Boca Raton, FL 2008, 3-32.
- [104] N.A. Peppas, R. Langer, New challenges in biomaterials, Science 263/5154 (1994) 1715-1720.
- [105] J.A. Hubbell, Biomaterials in tissue engineering, Biotechnology (N Y) 13/6 (1995) 565-576.
- [106] J.A. Hubbell, Bioactive biomaterials, Current Opinion in Biotechnology 10/2 (1999) 123-129.
- [107] K.E. Healy, A. Rezania, R.A. Stile, Designing biomaterials to direct biological responses, Annals of the New York Academy of Sciences 875 (1999) 24-35.
- [108] R. Langer, D.A. Tirrell, Designing materials for biology and medicine, Nature 428/6982 (2004) 487-492.
- [109] M.P. Lütolf, J.A. Hubbell, Synthetic biomaterials as instructive extracellular microenvironments for morphogenesis in tissue engineering, Nature Biotechnology 23/1 (2005) 47-55.
- [110] F. Yang, C.G. Williams, D.A. Wang, H. Lee, P.N. Manson, J. Elisseeff, The effect of incorporating RGD adhesive peptide in polyethylene glycol diacrylate hydrogel on osteogenesis of bone marrow stromal cells, Biomaterials 26/30 (2005) 5991-5998.
- [111] J. Elisseeff, A. Ferran, S. Hwang, S. Varghese, Z. Zhang, The role of biomaterials in stem cell differentiation: Applications in the musculoskeletal system, Stem Cells and Development 15/3 (2006) 295-303.
- [112] N.S. Hwang, M.S. Kim, S. Sampattavanich, J.H. Baek, Z. Zhang, J. Elisseeff, Effects of threedimensional culture and growth factors on the chondrogenic differentiation of murine embryonic stem cells, Stem Cells 24/2 (2006) 284-291.
- [113] C.J. Bettinger, J.T. Borenstein, R. Langer, Microfabrication Techniques in Scaffold Development, in: C.T. Laurencin, L.S. Nair, eds., Nanotechnology and Tissue Engineering: The Scaffold, CRC Press Taylor & Francis Group, Boca Raton, FL 2008.
- [114] C.E. Wilson, W.J. Dhert, C.A. van Blitterswijk, A.J. Verbout, J.D. De Bruijn, Evaluating 3D bone tissue engineered constructs with different seeding densities using the alamarBlue assay and the effect on in vivo bone formation, Journal of Materials Science. Materials in Medicine 13/12 (2002) 1265-1269.
- [115]M.C. Kruyt, J.D. De Bruijn, C.E. Wilson, F.C. Oner, C.A. van Blitterswijk, A.J. Verbout, W.J. Dhert, Viable osteogenic cells are obligatory for tissueengineered ectopic bone formation in goats, Tissue Engineering 9/2 (2003) 327-336.
- [116] J. Folkman, Tumor angiogenesis: Therapeutic implications, New England Journal of Medicine 285/21 (1971) 1182-1186.

- [117] D.J. Mooney, G. Organ, J.P. Vacanti, R. Langer, Design and fabrication of biodegradable polymer devices to engineer tubular tissues, Cell Transplant 3/2 (1994) 203-210.
- [118] G. Li, A.S. Virdi, D.E. Ashhurst, A.H. Simpson, J.T. Triffitt, Tissues formed during distraction osteogenesis in the rabbit are determined by the distraction rate: Localization of the cells that express the mRNAs and the distribution of types I and II collagens, Cell Biology International 24/1 (2000) 25-33.
- [119] J.E. Sanders, S.G. Malcolm, S.D. Bale, Y.N. Wang, S. Lamont, Prevascularization of a biomaterial using a chorioallontoic membrane, Microvascular Research 64/1 (2002) 174-178.
- [120] G.F. Muschler, C. Nakamoto, L.G. Griffith, Engineering principles of clinical cell-based tissue engineering, Journal of Bone and Joint Surgery 86-A/7 (2004) 1541-1558.
- [121] G. Helmlinger, F. Yuan, M. Dellian, R.K. Jain, Interstitial pH and pO₂ gradients in solid tumors in vivo: High-resolution measurements reveal a lack of correlation, Nature Medicine 3/2 (1997) 177-182.
- [122] M. Noga, A. Pawlak, B. Dybała, B. Dąbrowski, W. Swięszkowski, M. Lewandowska-Szumieł, Biological Evaluation of Porous Titanium Scaffolds (Ti-6Al-7Nb) with HAp/Ca-P surface seeded with Human Adipose Derived Stem Cells, International Scientific Conference E-MRS Fall Meeting, Warsaw, 2013.
- [123] Y. Khan, M.J. Yaszemski, A.G. Mikos, C.T. Laurencin, Tissue engineering of bone: material and matrix considerations, Journal of Bone & Joint Surgery 90/Suppl. 1 (2008) 36-42.
- [124] J. Rouwkema, N.C. Rivron, C.A. van Blitterswijk, Vascularization in tissue engineering, Trends Biotechnology 26/8 (2008) 434-441.
- [125]H. Bramfeldt, G. Sabra, V. Centis, P. Vermette, Scaffold Vascularization: A Challenge for Three-Dimensional Tissue Engineering, Current Medicinal Chemistry 17/33 (2010) 3944-3967.
- [126] R.K. Jain, P. Au, J. Tam, D.G. Duda, D. Fukumura, Engineering vascularized tissue, Nature Biotechnology 23 (2005) 821-823.
- [127] S. Rumiński, B. Ostrowska, W. Swięszkowski, M. Lewandowska-Szumieł, Human Adipose-Derived Stem Cells differentiate into osteoblast-like cells on ε-Polycaprolactone/Tricalcium Phosphate Composite Scaffolds, International Scientific Conference E-MRS Fall Meeting, Warsaw, 2013.
- [128] S. Rumiński, B. Ostrowska, W. Swięszkowski, M. Lewandowska-Szumieł, Osteogenic Differentiation of Human Adipose-Derived Stem Cells on Polycaprola-

- ctone/Tricalcium Phosphate Composite Scaffolds, Abstracts, European Chapter Meeting of the Tissue Engineering and Regenerative Medicine International Society, TERMIS, Istanbul, Turkey, 2013, 287.
- [129] M. Kolodziejczyk, I. Kalaszczynska, J. Sadlo, J. Kolmas, W. Kolodziejski, Ł. Pajchel, G. Kapron, G. Wilczynski, M. Lewandowska-Szumieł, Maturation of Newly Deposited Calcium-Phosphate Crystals in Human Adipose Derived Stem Cells Culture after Cell Differentiation to Osteoblast in vitro, Abstracts, European Chapter Meeting of the Tissue Engineering and Regenerative Medicine International Society, TERMIS, Istanbul, Turkey, 2013, 100.
- [130] M. Noga, A. Pawlak, B. Dybała, B. Dąbrowski, W. Swięszkowski, M. Lewandowska-Szumieł, Preparation and Evaluation of Biological Properties of Bioimplants Composed of Adipose Derived Stem Cells and Porous Titanium Scaffold (Ti-6Al-7Nb) with HAp/Ca-P Surface, Abstracts, TERMIS, Istanbul, Turkey, 2013, 733.
- [131]M. Karoluk, A. Pawlak, E. Chlebus, The use of incremental SLM technology in the process of Ti-6Al-7Nb titanium alloy manufacturing for biomedical applications, XI Konferencja Naukowa im. Prof. Dagmary Tejszerskiej, Ustroń, 2014, 53-54 (in Polish).
- [132] I.M. Wojak-Cwik, V. Hintze, M. Schnabelrauch, S. Moeller, P. Dobrzynski, E. Pamula, D. Scharnweber, Poly(L-lactide-co-glycolide) scaffolds coated with collagen and glycosaminoglycans: Impact on proliferation and osteogenic differentiation of human mesenchymal stem cells, Journal of Biomedical Materials Research Part A 101/11 (2013) 3109-3122.
- [133] P. Wilczek, M. Zembala, T. Cichoń, R. Smolarczyk, S. Szala, M. Zembala, Scaffold construction for effective transfer of cardiac stem cells to the damaged heart, Kardiochirurgia i Torakochirurgia Polska 9/2 (2012) 231-242.
- [134] E. Stodolak-Zych, A. Frączek-Szczypta, A. Wiecheć, M. Błażewicz, Nanocomposite Polymer Scaffolds for Bone Tissue Regeneration, Acta Physica Polonica A 121/2 (2012) 518-521.
- [135] M.T. Błażewicz, et al., Nanocomposite materials for regenerative medicine, Project N N507 463537, 2009-2012.
- [136] L. Rzeszutko, Z. Siudak, A. Włodarczak, A. Lekston, R. Depukat, A. Ochała, R.J. Gil, W. Balak, M. Marć, J. Kochman, W. Zasada, D. Dudek, Contemporary use of bioresorbable vascular scaffolds (BVS) in patients with stable angina and acute coronary syndromes. Polish National Registry, Kardiologia Polska 72/12 (2014) 1394-1399.

- [137] J. Street, D. Winter, J.H. Wang, A. Wakai, A. Mc-Guinness, H.P. Redmond, Is human fracture hematoma inherently angiogenic? Clinical Orthopaedics and Related Research 378 (2000) 224-237.
- [138] J.M. Karp, F. Sarraf, M.S. Shoichet, J.E. Davies, Fibrin-filled scaffolds for bone-tissue engineering: An in vivo study, Journal of Biomedical Materials Research Part A 71/1 (2004) 162-171.
- [139] K.F. Leong, C.M. Cheah, C.K. Chua, Solid freeform fabrication of three-dimensional scaffolds for engineering replacement tissues and organs, Biomaterials 24/13 (2003) 2363-2378.
- [140] L.S. Nair, C.T. Laurencin, Polymers as biomaterials for tissue engineering and controlled drug delivery, Advances in Biochemical Engineering, Biotechnology 102 (2006) 47-90.
- [141] J. Velema, D. Kaplan, Biopolymer-based biomaterials as scaffolds for tissue engineering, Advances in Biochemical Engineering, Biotechnology 102 (2006) 187-238.
- [142] J. Viola, B. Lal, O. Grad, The Emergence of Tissue Engineering as a Research Field. Arlington, The National Science Foundation, 2003, http://www.nsf.gov/pubs/2004/nsf0450/.
- [143] S.P. Bruder, D.J. Fink, A.I. Caplan, Mesenchymal stem cells in bone development, bone repair, and skeletal regeneration therapy, Journal of Cellular Biochemistry 56/3 (1994) 283-294.
- [144] J.E. Aubin, Bone stem cells, Journal of Cellular Biochemistry Suppl 30-31 (1998) 73-82.
- [145] M.J. Shamblott, J. Axelman, S. Wang, E.M. Bugg, J.W. Littlefield, P.J. Donovan, P.D. Blumenthal, G.R. Huggins, J.D. Gearhart, Derivation of pluripotent stem cells from cultured human primordial germ cells, Proceedings of the National Academy of Sciences USA 95/23 (1998) 13726-13731.
- [146] J.A. Thomson, J. Itskovitz-Eldor, S.S. Shapiro, M.A. Waknitz, J.J. Swiergiel, V.S. Marshall, J.M. Jones, Embryonic stem cell lines derived from human blastocysts, Science 282/5391 (1998) 1145-1147.
- [147] M.F. Pittenger, A.M. Mackay, S.C. Beck, R.K. Jaiswal, R. Douglas, J.D. Mosca, M.A. Moorman, D.W. Simonetti, S. Craig, D.R. Marshak, Multilineage potential of adult human mesenchymal stem cells, Science 284/5411 (1999) 143-147.
- [148] V. Sottile, A. Thomson, J. McWhir, In vitro osteogenic differentiation of human ES cells, Cloning Stem Cells 5/2 (2003) 149-155.
- [149] C.M. Cowan, Y.Y. Shi, O.O. Aalami, Y.F. Chou, C. Mari, R. Thomas, N. Quarto, C.H. Contag, B. Wu, M.T. Longaker, Adipose-derived adult stromal cells

- heal critical-size mouse calvarial defects, Nature Biotechnology 22/5 (2004) 560-567.
- [150] M.S. Kim, N.S. Hwang, J. Lee, T.K. Kim, K. Leong, M.J. Shamblott, J. Gearhart, J. Elisseeff, Musculoskeletal differentiation of cells derived from human embryonic germ cells, Stem Cells 23/1 (2005) 113-123.
- [151] W.S. Hwang, Y.J. Ryu, J.H. Park, E.S. Park, E.G. Lee, J.M. Koo, H.Y. Jeon, B.C. Lee, S.K. Kang, S.J. Kim, C. Ahn, J.H. Hwang, K.Y. Park, J.B. Cibelli, S.Y. Moon, Evidence of a pluripotent human embryonic stem cell line derived from a cloned blastocyst, Science 303/5664 (2004) 1669-1674.
- [152] R.P. Lanza, J.B. Cibelli, M.D. West, Prospects for the use of nuclear transfer in human transplantation, Nature Biotechnology 17/12 (1999) 1171-1174.
- [153] C.L. Cetrulo Jr., Cord-blood mesenchymal stem cells and tissue engineering, Stem Cell Reviews and Reports 2/2 (2006) 163-168.
- [154]D. Baksh, R. Yao, R.S. Tuan, Comparison of proliferative and multilineage differentiation potential of human mesenchymal stem cells derived from umbilical cord and bone marrow, Stem Cells 25/6 (2007) 1384-1392.
- [155] A.I. Caplan, S.P. Bruder, Mesenchymal stem cells: Building blocks for molecular medicine in the 21st century, Trends in Molecular Medicine 7/6 (2001) 259-264.
- [156] P.A. Zuk, M. Zhu, H. Mizuno, J. Huang, J.W. Futrell, A.J. Katz, P. Benhaim, H.P. Lorenz, M.H. Hedrick, Multilineage cells from human adipose tissue: Implications for cell-based therapies, Tissue Engineering 7/2 (2001) 211-228.
- [157] D. Baksh, J.E. Davies, P.W. Zandstra, Adult human bone marrow-derived mesenchymal progenitor cells are capable of adhesion-independent survival and expansion, Experimental Hematology 31/8 (2003) 723-732.
- [158] R. Izadpanah, C. Trygg, B. Patel, C. Kriedt, J. Dufour, J.M. Gimble, B.A. Bunnell, Biologic properties of mesenchymal stem cells derived from bone marrow and adipose tissue, Journal of Cellular Biochemistry 99/5 (2006) 1285-1297.
- [159] K. Le Blanc, L. Tammik, B. Sundberg, S.E. Haynesworth, O. Ringden, Mesenchymal stem cells inhibit and stimulate mixed lymphocyte cultures and mitogenic responses independently of the major histocompatibility complex, Scandinavian Journal of Immunology 57/1 (2003) 11-20.
- [160] S. Aggarwal, M.F. Pittenger, Human mesenchymal stem cells modulate allogeneic immune cell responses, Blood 105/4 (2005) 1815-1822.

- [161]B. Maitra, E. Szekely, K. Gjini, M.J. Laughlin, J. Dennis, S.E. Haynesworth, O.N. Koc, Human mesenchymal stem cells support unrelated donor hematopoietic stem cells and suppress T-cell activation, Bone Marrow Transplant 33/6 (2004) 597-604.
- [162] N. Dagalakis, J. Flink, P. Stasikelis, J.F. Burke, I.V. Yannas, Design of an artificial skin. Part III. Control of pore structure, Journal of Biomedical Materials Research 14/4 (1980) 511-528.
- [163] D.J. Mooney, D.F. Baldwin, N.P. Suh, J.P. Vacanti, R. Langer, Novel approach to fabricate porous sponges of poly(D,L-lactic-co-glycolic acid) without the use of organic solvents, Biomaterials 17/14 (1996) 1417-1422.
- [164] H.L. Wald, G. Sarakinos, M.D. Lyman, A.G. Mikos, J.P. Vacanti, R. Langer, Cell seeding in porous transplantation devices, Biomaterials 14/4 (1993) 270-278.
- [165] M.J. Lima, V.M. Correlo, R.L. Reis, Micro/nano replication and 3D assembling techniques for scaffold fabrication, Materials Science and Engineering C 42 (2014) 615-621.
- [166] G.J. Wang, C.L. Chen, S.H. Hsu, Y.L. Chiang, Bio-MEMS fabricated artificial capillaries for tissue engineering, Microsystem Technologies 12/1-2 (2005) 120-127.
- [167] C.Y. Tay, S.A. Irvine, F.Y.C. Boey, L.P. Tan, S. Venkatraman, Micro-/nano-engineered cellular responses for soft tissue engineering and biomedical applications, Small 7/10 (2011) 1361-1378.
- [168]E. Delamarche, A. Bernard, H. Schmid, B. Michel, H. Biebuyck, Patterned delivery of immunoglobulins to surfaces using microfluidic networks, Science 276/5313 (1997) 779-781.
- [169] J. Kim, H.N. Kim, Y. Lang, A. Pandit, Biologically inspired micro- and nanoengineering systems for functional and complex tissues, Tissue Engineering Part A 20/15-16 (2014) 2127-2130.
- [170]M. Schvartzman, S.J. Wind, Robust pattern transfer of nanoimprinted features for sub-5-nm fabrication, Nano Letters 9/10 (2009) 3629-3634.
- [171] S.Y. Chou, P.R. Krauss, W. Zhang, L. Guo, L. Zhuang, Sub-10 nm Imprint Lithography and Applications, Papers from the 41st International Conference on Electron, Ion, and Photon Beam Technology and Nanofabrication, Dana Point, California, USA, 1997, 2897-2904.
- [172] S. Zhang, L. Yan, M. Altman, M Lässle, H. Nugent, F. Frankel, D.A. Lauffenburger, G.M. Whitesides, A. Rich, Biological surface engineering: a simple system for cell pattern formation, Biomaterials 20/13 (1999) 1213-1220.

- [173] H. Cao, Z. Yu, J. Wang, J.O. Tegenfeldt, R.H. Austin, E. Chen, W. Wu, S.Y. Chou, Fabrication of 10 nm enclosed nanofluidic channels, Applied Physics Letters 81/1 (2002) 174-176.
- [174] S. Bose, S. Suguira, A. Bandyopadhyay, Processing of controlled porosity ceramic structures via fused deposition, Scripta Materialia 41/9 (1999) 1009-1014.
- [175] J. Darsell, S. Bose, H.L. Hosick, A. Bandyopadhyay, From CT scan to ceramic bone graft, Journal of the American Ceramic Society 86(7 (2003) 1076-1080.
- [176] D.W. Hutmacher, M. Sittinger, M.V. Risbud, Scaffold-based tissue engineering: rationale for computer-aided design and solid free-form fabrication systems. Trends in Biotechnology 22/7 (2004) 354-362.
- [177] E.M. Sachs, S.H. John, J.C. Michael, A.W. Paul, Three-dimensional printing techniques, Massachusetts Institute of Technology, U.S. Patent 5,204,055, 1993.
- [178] W.-Y. Yeong, C.-K. Chua, K.-F. Leong, M. Chandrasekaran, M.-W. Lee, Indirect fabrication of collagen scaffold based on inkjet printing technique, Rapid Prototyping Journal 12(4 (2006) 229-237.
- [179] T. Dutta Roy, J.L. Simon, J.L. Ricci, E.D. Rekow, V.P. Thompson, J.R. Parsons, Performance of hydroxyapatite bone repair scaffolds created via threedimensional fabrication techniques, Journal of Biomedical Materials Research Part A 67/4 (2003) 1228-1237.
- [180] A. Khalyfa, S. Vogt, J. Weisser, G. Grimm, A. Rechtenbach, W. Meyer, M. Schnabelrauch, Development of a new calcium phosphate powder-binder system for the 3D printing of patient specific implants, Journal of Materials Science. Materials in Medicine 18/5 (2007) 909-916.
- [181] I. Manjubala, A. Woesz, C. Pilz, M. Rumpler, N. Fratzl-Zelman, P. Roschger, J. Stampfl, P. Fratzl, Biomimetic mineral-organic composite scaffolds with controlled internal architecture, Journal of Materials Science. Materials in Medicine 16/12 (2005) 1111-1119.
- [182] E. Sachlos, N. Reis, C. Ainsley, B. Derby, J.T. Czernuszka, Novel collagen scaffolds with predefined internal morphology made by solid freeform fabrication, Biomaterials 24/8 (2003) 1487-1497.
- [183] M.J. Sawkins, K.M. Shakesheff, L.J. Bonassar, G.R. Kirkham, 3D Cell and Scaffold Patterning Strategies in Tissue Engineering, Recent Patents on Biomedical Engineering 6/1 (2013) 3-21.
- [184] M.N. Cooke, J.P. Fisher, D. Dean, C. Rimnac, A.G. Mikos, Use of stereolithography to manufacture

- critical-sized 3D biodegradable scaffolds for bone ingrowth, Journal of Biomedical Materials Research Part B: Applied Biomaterials 64B/2 (2003) 65-69.
- [185]K.W. Lee, S. Wang, B.C. Fox, E.L. Ritman, M.J. Yaszemski, L. Lu, Poly(propylene fumarate) bone tissue engineering scaffold fabrication using stereolithography: Effects of resin formulations and laser parameters, Biomacromolecules 8/4 (2007) 1077-1084
- [186]B. Dhariwala, E. Hunt, T. Boland, Rapid prototyping of tissue-engineering constructs, using photopolymerizable hydrogels and stereolithography, Tissue Engineering 10/9-10 (2004) 1316-1322.
- [187] K. Arcaute, B.K. Mann, R.B. Wicker, Stereolithography of three-dimensional bioactive poly (ethylene glycol) constructs with encapsulated cells, Annals of Biomedical Engineering 34/9 (2006) 1429-1441.
- [188] D.W. Hutmacher, T. Schantz, I. Zein, K.W. Ng, S.H. Teoh, K.C. Tan, Mechanical properties and cell cultural response of polycaprolactone scaffolds designed and fabricated via fused deposition modelling, Journal of Biomedical Materials Research 55/2 (2001) 203-216.
- [189]H.-T. Liao, Y.-Y. Chen, Y.-T. Lai, M.-F. Hsieh, C.-P. Jiang, The Osteogenesis of Bone Marrow Stem Cells on mPEG-PCL-mPEG/Hydroxyapatite Composite Scaffold via Solid Freeform Fabrication, BioMed Research International (2014) Article ID 321549.
- [190] M.E. Hoque, D.W. Hutmacher, W. Feng, S. Li, M.H. Huang, M. Vert, Y.S. Wong, Fabrication using a rapid prototyping system and in vitro characterization of PEG–PCL–PLA scaffolds for tissue engineering, Journal of Biomaterials Science, Polymer Edition 16/12 (2005) 1595-1610.
- [191] K.C. Ang, K.F. Leong, C.K. Chua, M. Chandrase-karan, Investigation of mechanical properties and porosity relationships fabricated porous structures, Rapid Prototyping Journal 12/2 (2006) 100-105.
- [192] J.J. Sun, C.J. Bae, Y.H. Koh, H.E. Kim, H.W. Kim, Fabrication of hydroxyapatite-poly(epsiloncaprolactone) scaffolds by a combination of the extrusion and bi-axial lamination processes, Journal of Materials Science. Materials in Medicine 18, (2007) 1017-1023.
- [193] S.S. Crump, Apparatus and method for creating three-dimensional objects, Stratasys Inc., U.S. Patent 5,121,329A, 1992.
- [194] L.A. Dobrzański, A. Achtelik-Franczak, Structure and properties of the microporous titanium scaffolds produced by selective laser sintering, prepared for print.

- [195] J.M. Williams, A. Adewunmi, R.M. Schek, C.L. Flanagan, P.H. Krebsbach, S.E. Feinberg, S.J. Hollister, S. Das, Bone tissue engineering using polycaprolactone scaffolds fabricated via selective laser sintering, Biomaterials 26/23 (2005) 4817-4827.
- [196] K.H. Tan, C.K. Chua, K.F. Leong, C.M. Cheah, W.S. Gui, W.S. Tan, F.E. Wiria, Selective laser sintering of biocompatible polymers for applications in tissue engineering, Bio-medical Materials and Engineering 15/1-2 (2005) 113-124.
- [197] C. Shuai, C. Gao, Y. Nie, H. Hu, Y. Zhou, S. Peng, Structure and properties of nano-hydroxypatite scaffolds for bone tissue engineering with a selective laser sintering system, Nanotechnology 22/28 (2011) 285703.
- [198] C.K. Chua, K.F. Leong, K.H. Tan, F.E. Wiria, C.M. Cheah, Development of tissue scaffolds using selective laser sintering of polyvinyl alcohol=hydroxyapatite biocomposite for craniofacial and joint defects, Journal of Materials Science. Materials in Medicine 15/10 (2004) 1113-1121.
- [199] F.E. Wiria, K.F. Leong, C.K. Chua, Y. Liu, Polyepsilon-caprolactone=hydroxyapatite for tissue engineering scaffold fabrication via selective laser sintering, Acta Biomaterialia 3/1 (2007) 1-12.
- [200] R. Murugan, S. Ramakrishna, Nano-featured scaffolds for tissue engineering: A review of spinning methodologies, Tissue Engineering 12/3 (2006) 435-447.
- [201] T.J. Sill, H.A. von Recum, Electrospinning: Applications in drug delivery and tissue engineering, Biomaterials 29/13 (2008) 1989-2006.
- [202] J.A. Matthews, G.E. Wnek, D.G. Simpson, G.L. Bowlin, Electrospinning of collagen nanofibers, Biomacromolecules 3/2 (2002) 232-238.
- [203] F. Yang, R. Murugan, S. Wang, S. Ramakrishna, Electrospinning of nano=micro scale poly(L-lactic acid) aligned fibers and their potential in neural tissue engineering, Biomaterials 26/15 (2005) 2603-2610.
- [204] R. Murugan, S. Ramakrishna, Design strategies of tissue engineering scaffolds with controlled fiber orientation, Tissue Engineering 13/8 (2007) 1845-1866.
- [205] J.D. Hartgerink, E. Beniash, S.I. Stupp, Self-assembly and mineralization of peptide-amphiphile nanofibers, Science 294/5547 (2001) 1684-1688.
- [206] J.D. Hartgerink, E. Beniash, S.I. Stupp, Peptideamphiphile nanofibers: A versatile scaffold for the preparation of self-assembling materials, Proceedings of the National Academy of Sciences of the USA 99/8 (2002) 5133-5138.

- [207] E. Beniash, J.D. Hartgerink, H. Storrie, J.C. Stendahl, S.I. Stupp Self-assembling peptide amphiphile nanofiber matrices for cell entrapment, Acta Biomaterialia 1/4 (2005) 387-397.
- [208] S. Zhang, F. Gelain, X. Zhao, Designer self-assembling peptide nanofiber scaffolds for 3D tissue cell cultures, Seminars in Cancer Biology 15/5 (2005) 413-420.
- [209] F. Gelain, A. Horii, S. Zhang, Designer self-assembling peptide scaffolds for 3-d tissue cell cultures and regenerative medicine, Macromolecular Bioscience 7/5 (2007) 544-551.
- [210] S.H. Um, J.B. Lee, N. Park, S.Y. Kwon, C.C. Umbach, D. Luo, Enzyme-catalysed assembly of DNA hydrogel, Nature Materials 5/10 (2006) 797-801.
- [211] J.A. Hunt, R. Chen, T. van Veen, N. Bryan, Hydrogels for tissue engineering and regenerative medicine, Journal of Materials Chemistry B 2 (2014) 5319-5338.
- [212] J. Guan, Y. Hong, Z. Ma, W.R. Wagner, Protein-reactive, thermoresponsive copolymers with high flexibility and biodegradability, Biomacromolecules 9/4 (2008) 1283-1292.
- [213]S. Qin, Y. Geng, D.E. Discher, S. Yang, Temperature-Controlled Assembly and Release from Polymer Vesicles of Poly(ethylene oxide)-block- poly(*N*-isopropylacrylamide), Advanced Materials 18/21 (2006) 2905-2909.
- [214] R. Liu, M. Fraylich, B.R. Saunders, Thermoresponsive copolymers: from fundamental studies to applications, Colloid and Polymer Science 287 (2009) 627-643.
- [215] S. Ohya, Y. Nakayama, T. Matsuda, In vivo evaluation of poly(N-isopropylacrylamide) (PNIPAM)-grafted gelatin as an in situ-formable scaffold, Journal of Artificial Organs 7/4 (2004) 181-186.
- [216]H. Tan, C.R. Chu, K.A. Payne, K.G. Marra, Injectable in situ forming biodegradable chitosan–hyaluronic acid based hydrogels for cartilage tissue engineering, Biomaterials 30/13 (2009) 2499-2506.
- [217] L.Q. Wang, K. Tu, Y. Li, J. Zhang, L. Jiang, Z. Zhang, Synthesis and characterization of temperature responsive graft copolymers of dextran with poly(*N*-isopropylacrylamide), Reactive and Functional Polymers 53 (2002) 19-27.
- [218] S.B. Lee, D.I. Ha, S.K. Cho, S.J. Kim, Y.M. Lee, Temperature/pH-sensitive comb-type graft hydrogels composed of chitosan and poly(*N*-isopropylacrylamide), Journal of Applied Polymer Science 92/4 (2004) 2612-2620.
- [219] B.K. Lau, Q.Q. Wang, W. Sun, L. Li, Micellization to Gelation of a Triblock Copolymer in Water: Thermo-

- reversibility and Scaling, Journal of Polymer Science Part B: Polymer Physics 42 (2004) 2014-2025.
- [220] B. Jeong, Y.H. Bae, S.W. Kim, Thermoreversible Gelation of PEG-PLGA-PEG Triblock Copolymer Aqueous Solutions, Macromolecules 32/21 (1999) 7064-7069.
- [221] C. Hiemstra, Z.Y. Zhong, L.B. Li, P.J. Dijkstra, J. Feijen, In-Situ Formation of Biodegradable Hydrogels by Stereocomplexation of PEG-(PLLA)₈ and PEG-(PDLA)₈ Star Block Copolymers, Biomacromolecules 7/10 (2006) 2790-2795.
- [222] W.S. Shim, J.H. Kim, H. Park, K. Kim, I.C. Kwon, D.S. Lee, Biodegradability and biocompatibility of a pH- and thermo-sensitive hydrogel formed from a sulfonamide-modified poly(ε-caprolactone-co-lactide)–poly(ethylene glycol)–poly(ε-caprolactone-co-lactide) block copolymer, Biomaterials 27/30 (2006) 5178-5185.
- [223] C.Y. Gong, S.A. Shi, P.W. Dong, B. Kan, M.L. Gou, X.H. Wang, X.Y. Li, F. Luo, X. Zhao, Y.Q. Wei, Z.Y. Qian, Synthesis and characterization of PEG-PCL-PEG thermosensitive hydrogel, International Journal of Pharmaceutics 365/1-2 (2009) 89-99.
- [224] K. Park, H.H. Jung, J.S. Son, J.-W. Rhie, K.D. Park, K.-D. Ahn, D.K. Han, Thermosensitive and celladhesive pluronic hydrogels for human adiposederived stem cells, Key Engineering Materials 342-343 (2007) 301-304.
- [225] K. Kurata, A. Dobashi, Novel Temperature- and pH-Responsive Linear Polymers and Crosslinked Hydrogels Comprised of Acidic L-α-Amino Acid Derivatives, Journal of Macromolecular Science, Part A. Pure and Applied Chemistry 41/2 (2004) 143-164.
- [226] K. Nagase, J. Kobayashi, A. Kikuchi, Y. Akiyama, H. Kanazawa, T. Okano, Preparation of thermoresponsive cationic copolymer brush surfaces and application of the surface to separation of biomolecules, Biomacromolecules 9/4 (2008) 1340-1347.
- [227] Y. Loo, S. Zhang, C.A.E. Hauser, From short peptides to nanofibers to macromolecular assemblies in biomedicine, Biotechnol Adv 30(3 (2012) 593-603.
- [228] C. Xu, J. Kopecek, Self-assembling hydrogels, Polymer Bulletin 58 (2007) 53-63.
- [229] S. Zhang, Fabrication of novel biomaterials through molecular self-assembly, Nature Biotechnology 21/10 (2003) 1171-1178.
- [230]S.A. Gabriel, C. Catherine, N.L. Krista, E. Beniash, D.A. Harrington, J.A. Kessler, S.I. Stupp, Selective Differentiation of Neural Progenitor Cells by High-Epitope Density Nanofibers, Science 303/5662 (2004) 1352-1355.

- [231] M.A. Bokhari, G. Akay, S. Zhang, M.A. Birch, The enhancement of osteoblast growth and differentiation in vitro on a peptide hydrogel-polyHIPE polymer hybrid material, Biomaterials 26/25 (2005) 5198-5208.
- [232] R. Chen, J.A. Hunt, Biomimetic materials processing for tissue-engineering processes, Journal of Materials Chemistry 17/38 (2007) 3974-3979.
- [233] H. Lihong, E.S. Read, S.P. Armes, D.J. Adams, Direct Synthesis of Controlled-Structure Primary Amine-Based Methacrylic Polymers by Living Radical Polymerization, Macromolecules 40/13 (2007) 4429-4438.
- [234] Q. Yu, F. Zeng, S. Zhu, Atom Transfer Radical Polymerization of Poly(ethylene glycol) Dimethacrylate, Macromolecules 34/6 (2001) 1612-1618.
- [235] J.A. Killion, L.M. Geever, D.M. Devine, L. Grehan, J.E. Kennedy, C.L. Higginbotham, Modulating the mechanical properties of photopolymerised polyethylene glycol-polypropylene glycol hydrogels for bone regeneration, Journal of Materials Science 47/18 (2012) 6577-6585.
- [236] C. Ye, Z.H. Li, D. Li, C.Y. Gao, Fabrication and mineralization of poly(propylene fumarate)/hydroxyapatite porous hydrogels, Acta Polymerica Sinica 10 (2012) 1143-1150.
- [237]J.H. Hui, X. Ren, M.H. Afizah, K.S. Chian, A.G. Mikos, Oligo[poly(ethylene glycol)fumarate] Hydrogel Enhances Osteochondral Repair in Porcine Femoral Condyle Defects, Clinical Orthopaedics 471/4 (2013) 1174-1185.
- [238] J.S. Choi, H.S. Yoo, Pluronic/chitosan hydrogels containing epidermal growth factor with wound-adhesive and photo-crosslinkable properties, Journal of Biomedical Materials Research Part A 95/2 (2010) 564-573.
- [239] E.A. Kamoun, H. Menzel, Crosslinking behavior of dextran modified with hydroxyethyl methacrylate upon irradiation with visible light Effect of concentration, coinitiator type, and solvent, Journal of Applied Polymer Science 117/6 (2010) 3128-3138.
- [240] S. Ibrahim, C.R. Kothapalli, Q.K. Kang, A. Ramamurthi, Characterization of glycidyl methacrylate Crosslinked hyaluronan hydrogel scaffolds incorporating elastogenic hyaluronan oligomers, Acta Biomaterialia 7/2 (2011) 653-665.
- [241] A.D. Rouillard, C.M. Berglund, J.Y. Lee, W.J. Polacheck, Y. Tsui, L.J. Bonassar, B.J. Kirby, Methods for Photocrosslinking Alginate Hydrogels Scaffolds with High Cell Viability, Tissue Engineering Part C 17/2 (2011) 173-179.
- [242] D.J. Overstreet, D. Dutta, S.E. Stabenfeldt, B.L. Vernon, Injectable hydrogels, Journal of Polymer Science Part B: Polymer Physics 50/13 (2012) 881-903.

- [243] M.P. Lütolf, G.P. Raeber, A.H. Zisch, T. Nicola, J.A. Hubell, Cell-Responsive Synthetic Hydrogels, Advanced Materials 15/11 (2003) 888-892.
- [244] X.Z. Shu, K. Ghosh, Y. Liu, F.S. Palumbo, Y. Luo, R.A. Clark, G.D. Prestwich, Attachment and spreading of fibroblasts on an RGD peptide-modified injectable hyaluronan hydrogel, Journal of Biomedical Materials Research Part A 68/2, (2004) 365-375.
- [245] J. Maia, L. Ferreira, R. Carvalho, M.A. Ramos, M.H. Gil, Synthesis and characterization of new injectable and degradable dextran-based hydrogels, Polymer 46/23 (2005) 9604-9614.
- [246] K.K. Nishi, A. Jayakrishnan, Preparation and in vitro evaluation of primaquine-conjugated gum arabic microspheres, Biomacromolecules 5/4 (2004) 1489-1495.
- [247] D.A. Wang, S. Varghese, B. Shama, I. Strehin, S. Fermanian, J. Gorham, D.H. Fairbrother, B. Cascio, J.H. Elisseeff, Multifunctional chondroitin sulphate for cartilage tissue-biomaterial integration, Nature Materials 6/5 (2007) 385-392.
- [248] J.J. Sperinde, L.G. Griffith, Control and prediction of gelation kinetics in enzymatically cross-linked poly-(ethylene glycol) hydrogels, Macromolecules 33/15 (2000) 5476-5480.
- [249] B.J. Ryan, N. Carolan, C. O'Fagain, Horseradish and soybean peroxidases: comparable tools for alternative niches? Trends in Biotechnology 24/8 (2006) 355-363.
- [250] L.S. Moreira Teixeira, J. Feijen, C.A. van Blitterswijk, P.J. Dijkstra, M. Karperien, Enzyme-catalyzed crosslinkable hydrogels: emerging strategies for tissue engineering, Biomaterials 33/5 (2012) 1281-1290.
- [251] R. Jin, L.S. Moreira Teixeira, P.J. Dijkstra, Z. Zhong, C.A. van Blitterswijk, M. Karperien, J. Feijen, Enzymatically crosslinked dextran-tyramine hydrogels as injectable scaffolds for cartilage tissue engineering, Tissue Engineering Part A 16/8 (2010) 2429-2440.
- [252] J.W.H. Wennink, K. Niederer, A.I. Bochyńska, L.S. Moreira Teixeira, M. Karperien, J. Feijen, P.J. Dijkstra, Injectable Hydrogels by Enzymatic Co-Crosslinking of Dextran and Hyaluronic Acid Tyramine Conjugates, Macromolecular Symposia 309-310/1 (2011) 213-221.
- [253] S. Sakai, K. Kawakami, Both ionically and enzymatically crosslinkable alginate-tyramine conjugate as materials for cell encapsulation, Journal of Biomedical Materials Research Part A 85/2 (2008) 345-351.
- [254] S. Sakai, Y. Ogushi, K. Kawakami, Enzymatically crosslinked carboxymethylcellulose-tyramine conjugate hydrogel: cellular adhesiveness and feasibility for cell sheet technology, Acta Biomaterialia 5/2 (2009) 554-559.

- [255] A.A. Amini, L.S. Nair, Enzymatically cross-linked injectable gelatin gel as osteoblast delivery vehicle, Journal of Bioactive and Compatible Polymers 27/4 (2012) 342-355.
- [256] C. Fernandez, C.M. Hattan, R.J. Kerns, Semi-synthetic heparin derivatives: chemical modifications of heparin beyond chain length, sulfate substitution pattern and *N*-sulfo/*N*-acetyl groups, Carbohydrate Research 341/10 (2006) 1253-1265.
- [257] K.M. Park, Y.M. Shin, Y.K. Joung, H. Shin, K.D. Park, In situ forming hydrogels based on tyramine conjugated 4-arm-PPO-PEO via enzymatic oxidative reaction, Biomacromolecules 11/3 (2010) 706-712.
- [258] J.S. Patil, M.V. Kamalapur, S.C. Marapur, D.V. Kadam, Ionotropic gelation and polyelectrolyte complexation: the novel techniques to design hydrogel particulate sustained, modulated drug delivery system: A review, Digest Journal of Nanomaterials and Biostructures 5/1 (2010) 241-248.
- [259] K.E. Crompton, J.D. Goud, R.V. Bellamkonda, T.R. Gengenbach, D.I. Finkelstein, M.K. Horne, J.S. Forsythe, Polylysine-functionalised thermoresponsive chitosan hydrogel for neural tissue engineering, Biomaterials 28/3 (2007) 441-449.
- [260] J. Berger, M. Reist, J.M. Mayer, O. Felt, N.A. Peppas, R. Gurny, Structure and interactions in covalently and ionically crosslinked chitosan hydrogels for biomedical applications, European Journal of Pharmaceutics and Biopharmaceutics 57/1 (2004) 19-34.
- [261] J.K. Tessmar, A.M. Gopferich, Customized PEGderived copolymers for tissue-engineering applications, Macromolecular Bioscience 7/1 (2007) 23-39.
- [262] J. Baier Leach, K.A. Bivens, C.W. Patrick Jr., C.E. Schmidt, Photocrosslinked hyaluronic acid hydrogels: Natural, biodegradable tissue engineering scaffolds, Biotechnology and Bioengineering 82/5 (2003) 578-589.
- [263] J.L. Young, J. Tuler, R. Braden, P. Schüp-Magoffin, J. Schaefer, K. Kretchmer, K.L. Christman, A.J. Engler, In vivo response to dynamic hyaluronic acid hydrogels, Acta Biomaterialia 9/7 (2013) 7151-7157.
- [264] X.Z. Shu, Y. Liu, F.S. Palumbo, Y. Luo, G.D. Prestwich, In situ crosslinkable hyaluronan hydrogels for tissue engineering, Biomaterials 25/7-8 (2004) 1339-1348.
- [265] N.N. Fathima, B. Madhan, J.R. Rao, B.U. Nair, T. Ramasami Interaction of aldehydes with collagen: effect on thermal, enzymatic and conformational stability, International Journal of Biological Macromolecules 34/4 (2004) 241-247.

- [266] D. MacAya, K.K. Ng, M. Spector, Injectable Collagen-Genipin Gel for the Treatment of Spinal Cord Injury: In Vitro Studies, Advanced Functional Materials 21/24 (2011) 4788-4797.
- [267] Y.J. Hwang, J.G. Lyubovitsky, The structural analysis of three-dimensional fibrous collagen hydrogels by Raman microspectroscopy, Biopolymers 99/6 (2013) 349-356.
- [268] J.B. Leach, K.A. Bivens, C.N. Collins, C.E. Schmidt, Development of photocrosslinkable hyaluronic acidpolyethylene glycol-peptide composite hydrogels for soft tissue engineering, Journal of Biomedical Materials Research Part A 70/1 (2004) 74-82.
- [269] J. Berger, M. Reist, J.M. Mayer, O. Felt, R. Gurny, Structure and interactions in chitosan hydrogels formed by complexation or aggregation for biomedical applications, European Journal of Pharmaceutics and Biopharmaceutics 57/1 (2004) 35-52.
- [270] Y. Hong, H. Song, Y. Gong, Z. Mao, C. Gao, J. Shen, Covalently crosslinked chitosan hydrogel: Properties of in vitro degradation and chondrocyte encapsulation, Acta Biomaterialia 3/1 (2007) 23-31.
- [271] A. Lahiji, A. Sohrabi, D.S. Hungerford, C.G. Frondoza, Chitosan supports the expression of extracellular matrix proteins in human osteoblasts and chondrocytes, Journal of Biomedical Materials Research 51/4 (2000) 586-595.
- [272] R. Jin, C. Hiemstra, Z. Zhong, J. Feijen, Enzyme-mediated fast in situ formation of hydrogels from dextran-tyramine conjugates, Biomaterials 28/18 (2007) 2791-2800.
- [273] J.M. Jukes, L.J. van der Aa, C. Hiemstra, T. van Veen, P.J. Dijkstra, Z.Y. Zhong, J. Feijen, A Newly Developed Chemically Crosslinked Dextran— Poly(Ethylene Glycol) Hydrogel for Cartilage Tissue Engineering, Tissue Engineering Part A 16/2 (2010) 565-573.
- [274] A. Mosahebi, M. Simon, M. Wiberg, G. Terenghi, A novel use of alginate hydrogel as Schwann cell matrix, Tissue Engineering 7/5 (2001) 525-534.
- [275]B.G. Ballios, M.J. Cooke, D. van der Kooy, M.S. Shoichet, A hydrogel-based stem cell delivery system to treat retinal degenerative diseases, Biomaterials 31/9 (2010) 2555-2564.
- [276] U. Noth, K. Schupp, A. Heymer, S. Kall, F. Jakob, N. Schutze, B. Baumann, T. Barthel, J. Eulert, C. Hendrich, Anterior cruciate ligament constructs fabricated from human mesenchymal stem cells in a collagen type I hydrogel, Cytotherapy 7/5 (2005) 447-455.

- [277] J. Gao, R. Liu, J. Wu, Z. Liu, J. Li, J. Zhou, T. Hao, Y. Wang, Z. Du, C. Duan, C. Wang, The use of chitosan based hydrogel for enhancing the therapeutic benefits of adipose-derived MSCs for acute kidney injury, Biomaterials 33/14 (2012) 3673-3681.
- [278] S.L. Hume, S.M. Hoyt, J.S. Walker, B.V. Sridhar, J.F. Ashley, C.N. Bowman, S.J. Bryant, Alignment of multi-layered muscle cells within three-dimensional hydrogel macrochannels, Acta Biomaterialia 8/6 (2012) 2193-2202.
- [279] S. Shinohara, T. Kihara, S. Sakai, M. Matsusaki, M. Akashi, M. Taya, J. Miyake, Fabrication of in vitro three-dimensional multilayered blood vessel model using human endothelial and smooth muscle cells and high-strength PEG hydrogel, Journal of Bioscience and Bioengineering 116/2 (2013) 231-234.
- [280] Y. Liu, M.B. Chan-Park, Hydrogel based on interpenetrating polymer networks of dextran and gelatin for vascular tissue engineering. Biomaterials 30/2 (2009) 196-207.
- [281] T. Sawada, K. Tsukada, K. Hasegawa, Y. Ohashi, Y. Udagawa, V. Gomel, Cross-linked hyaluronate hydrogel prevents adhesion formation and reformation in mouse uterine horn model, Human Reproduction 16/2 (2001) 353-356.
- [282] Y. Yeo, C.B. Highley, E. Bellas, T. Ito, R. Marini, R. Langer, D.S. Kohane, In situ cross-linkable hyaluronic acid hydrogels prevent post-operative abdominal adhesions in a rabbit model, Biomaterials 27/27 (2006) 4698-4705.
- [283] D.L. Hern, J.A. Hubbell, Incorporation of adhesion peptides into nonadhesive hydrogels useful for tissue resurfacing, Journal of Biomedical Materials Research 39/2 (1998) 266-276.
- [284] J.A. Rowley, G. Madlambayan, D.J. Mooney, Alginate hydrogels as synthetic extracellular matrix materials, Biomaterials 20/1 (1999) 45-53.
- [285]T. Kaneko, S. Tanaka, A. Ogura, M. Akashi, Tough, thin hydrogel membranes with giant crystalline domains composed of precisely synthesized macromolecules, Macromolecules 38/11 (2005) 4861-4867.
- [286] D.J. Odde, M.J. Renn, Laser-guided direct writing of living cells, Biotechnology and Bioengineering 67/3 (2000) 312-318.
- [287] Y. Nahmias, R.E. Schwartz, C.M. Verfaillie, D.J. Odde, Laser-guided direct writing for threedimensional tissue engineering, Biotechnology and Bioengineering 92/2 (2005) 129-136.
- [288] V. Mironov, T. Trusk, V. Kasyanov, S. Little, R. Swaja, R. Markwald, Biofabrication: a 21st century manufacturing paradigm, Biofabrication 1/2 (2009) 1-16.

- [289] V. Mironov, T. Boland, T. Trusk, G. Forgacs, R. Markwald, Organ printing: computer-aided jet-based 3D tissue engineering, Trends in Biotechnology 21/4 (2003) 157-161.
- [290] T. Boland, V. Mironov, A. Gutowska, E.A. Roth, R.R. Markwald, Cell and organ printing 2: Fusion of cell aggregates in three-dimensional gels, The Anatomical Record. Part A, Discoveries in Molecular, Cellular, and Evolutionary Biology 272/2 (2003) 497-502.
- [291] R. Landers, R. Mülhaupt, Desktop manufacturing of complex objects, prototypes and biomedical scaffolds by means of computer-assisted design combined with computer-guided 3D plotting of polymers and reactive oligomers, Macromolecular Materials and Engineering 282/1 (2000) 17-21.
- [292] W. Tan, T.A. Desai, Layer-by-layer microfluidics for biomimetic three-dimensional structures, Biomaterials 25/7-8 (2004) 1355-1364.
- [293] D.R. Albrecht, G.H. Underhill, T.B. Wassermann, R.L. Sah, S.N. Bhatia, Probing the role of multicellular organization in three-dimensional microenvironments, Nature Methods 3/5 (2006) 369-375.
- [294]S. Writers, Invetech helps bring bio-printers to life, LifeScientist, 2009, http://lifescientist.com.au/ content/biotechnology/news/invetech-helps-bringbio-printers-to-life-413047968.
- [295] S. Bhatia, M. Birchall, et al., 3D-printed sugar network to help grow artificial liver, BBC, 2012, http://www.bbc.com/news/technology-18677627.
- [296] L.E. Bertassoni, M. Cecconi, V. Manoharan, M. Nikkhah, J. Hjortnaes, A.L. Cristino, G. Barabaschi, D. Demarchi, M.R. Dokmeci, Y. Yang, A. Khademhosseini, Hydrogel bioprinted microchannel networks for vascularization of tissue engineering constructs, Lab on a Chip 14/13 (2014) 2202-2211.
- [297] T.A. Campbell, R. Reid et al., 3D Printing: Challenges and Opportunities for International Relations, Transcript, Council on Foreign Relations, CFR.org, 2013, http://www.cfr.org/technology-and-science/3d-printing-challenges-opportunities-international-relations/-p31709.
- [298] J.T. Quigley, Chinese Scientists Are 3D Printing Ears and Livers – With Living Tissue, Tech Biz, The Diplomat, 2013, http://thediplomat.com/2013/08/chinese-scientists-are-3d-printing-ears-and-liverswith-living-tissue/.
- [299] How do they 3D print kidney in China, 3Ders.org, 2013, http://www.3ders.org/articles/20130815-how-do-they-3d-print-kidney-in-china.html.

- [300]M. Littre, Humans could be fitted with kidneys made on 3D PRINTERS thanks to Australian researchers who have already grown miniature organs in labs, by K. Lyons, DailyMailOnline, 2014, http://www.dailymail.co.uk/sciencetech/article-2637158/Humans-fitte d-kidneys-3D-printers.html.
- [301] J. Hoying et al., New 3D bioprinter to reproduce human organs, change the face of healthcare: The inside story, by L. Gilpin, TechRepublic, 2014, http://www.techrepublic.com/article/new-3d-bioprin ter-to-reproduce-human-organs/.
- [302] D. Lambrick, World Artificial Organs Market by 2017, MarketandMarkets, 2014, http://www.powershow.com/view0/608c4e-YjNiM/World_Artificial_Organs_Market_by_2017_powerpoint_ppt_presentation
- [303] Medical Bionic Implant (Artificial Organs) Market (Vision Bionics/Bionic Eye, Brain Bionics, Heart Bionics/Artificial Heart, Orthopedic Bionics and Ear Bionics) Trends and Global Forecasts to 2017, MarketsandMarkets, 2012, http://www.marketsandmarkets.com/Market-Reports/medical-bionic-implant -market-908.html.

- [304] Orthopedic Trauma Fixation Devices Market Global Forecast, Market Share, Size, Growth and Industry Analysis 2014 2020, Transparency Market Research, 2014, http://www.transparencymarket research.com/orthopedic-trauma-fixation-device-market.html.
- [305] Orthopedic Soft Tissue Repair Market (Surgical Procedures ACL/PCL Reconstruction, Meniscal Repair, Rotator Cuff Repair, Hip Arthroscopy, Biceps Tenodesis and Shoulder Labrum Repair) Global Industry Analysis, Size, Share, Growth, Trends and Forecast, 2013 2019, Transparency Market Research, 2014, http://www.transparency marketresearch.com/soft-tissue-repair-sports-medici ne.html.
- [306] 3D Printing in Medical Applications Market (Medical Implants (Dental, Orthopedic, Cranio-maxillofacial), Surgical Guides, Surgical Instruments, Bioengineered Products) - Global Industry Analysis, Size, Share, Growth, Trends and Forecast, 2013 -2019, Transparency Market Research, 2014, http://www.transparencymarketresearch.com/3d-Printing-medical-applications.html.